

**COPY**

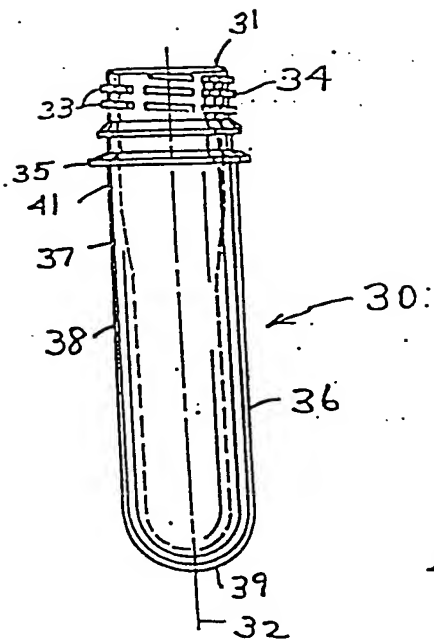


Fig. 1

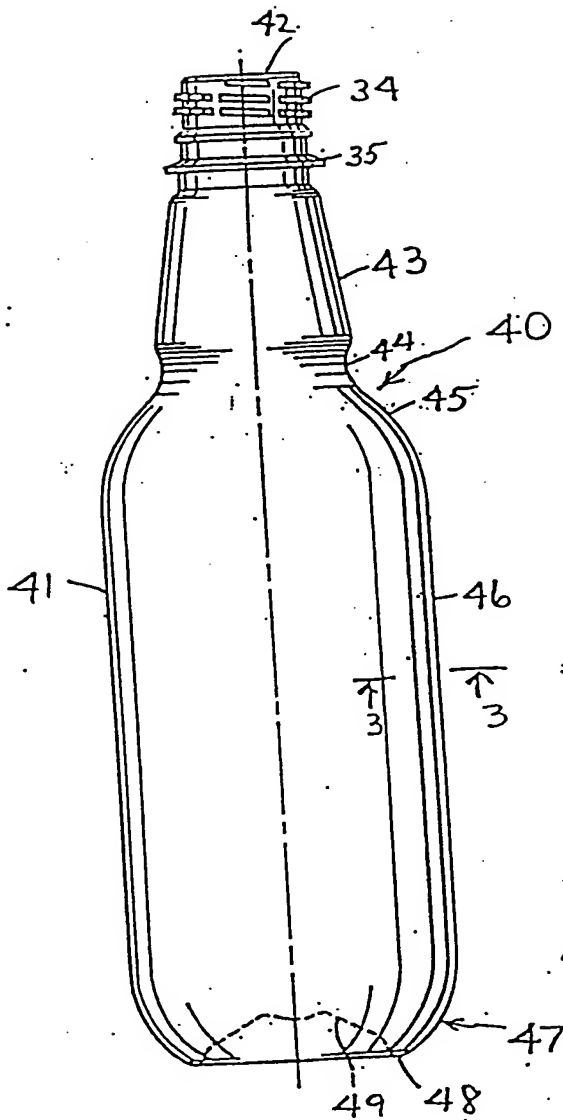


Fig. 2

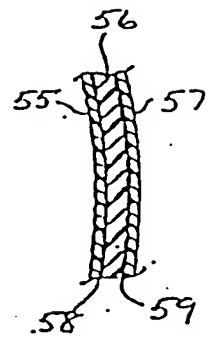
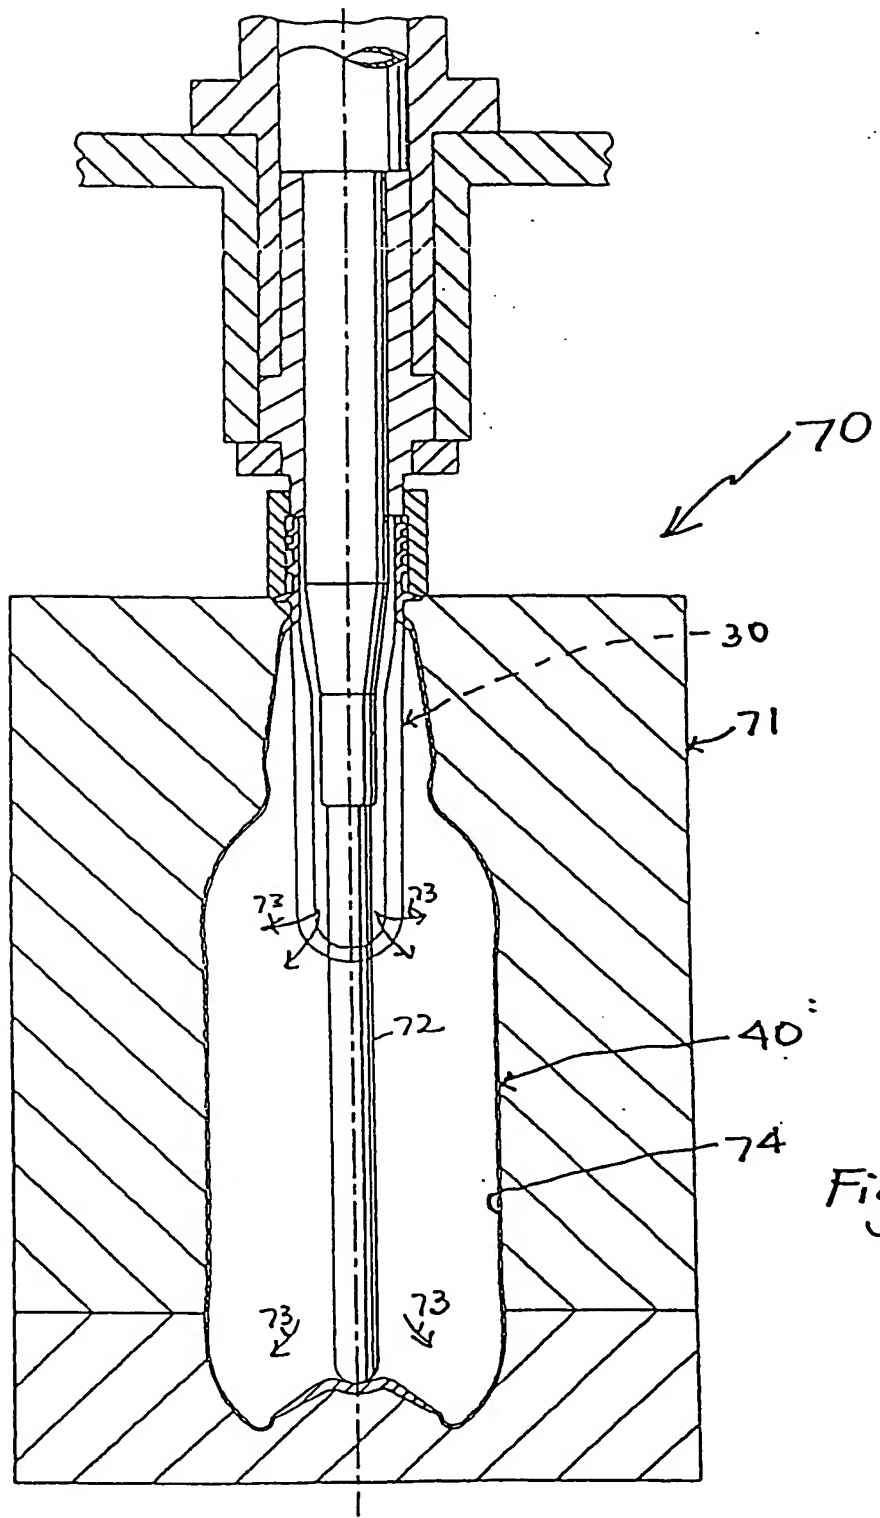


Fig. 3



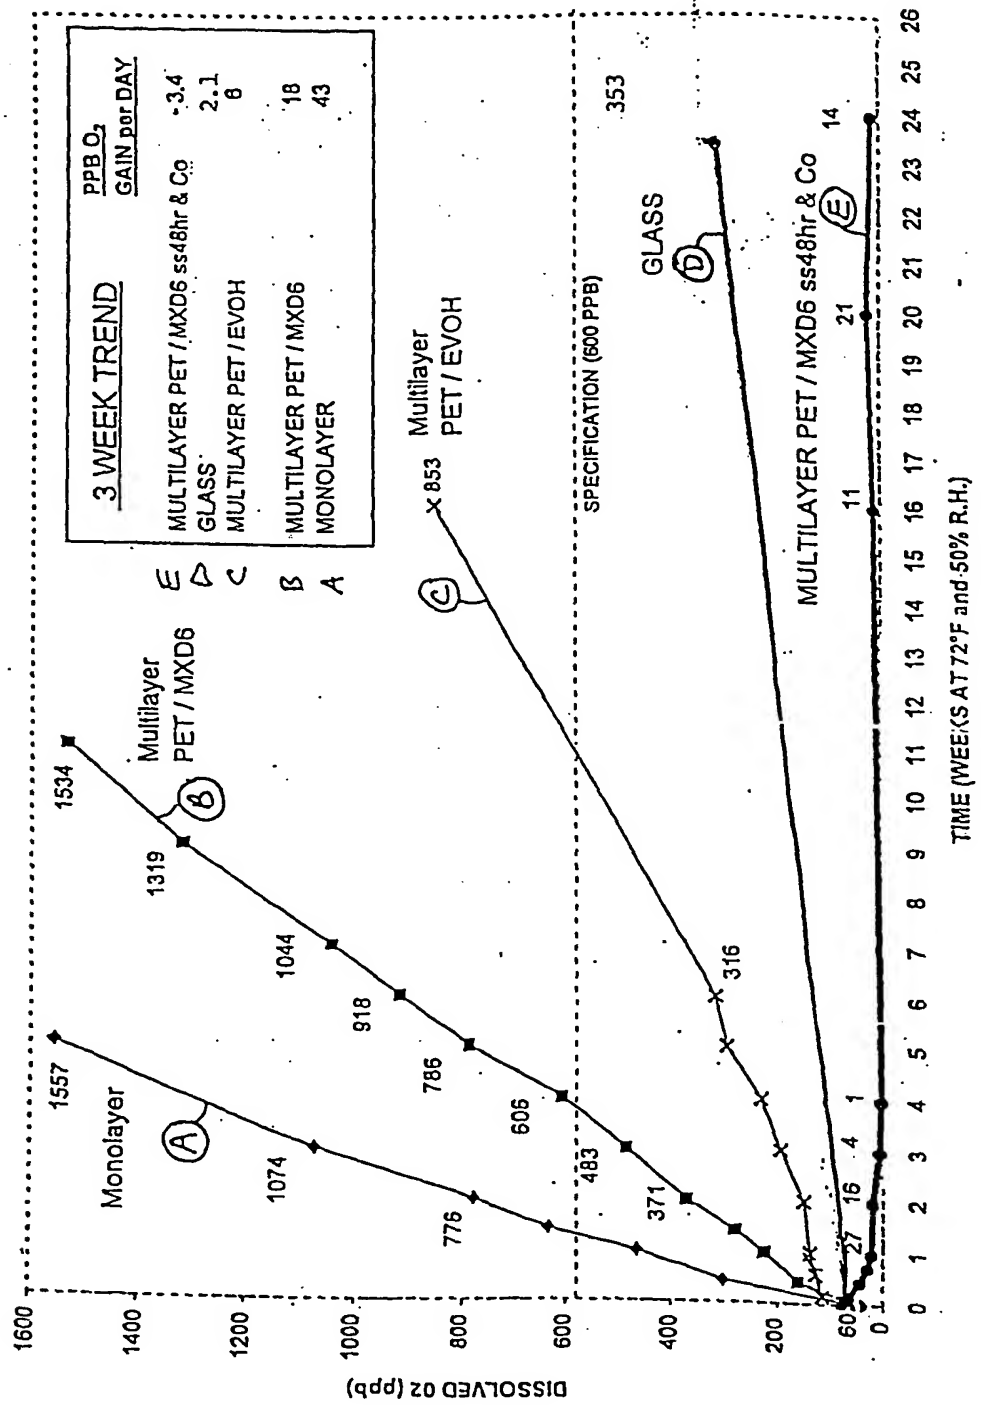


Fig. 5

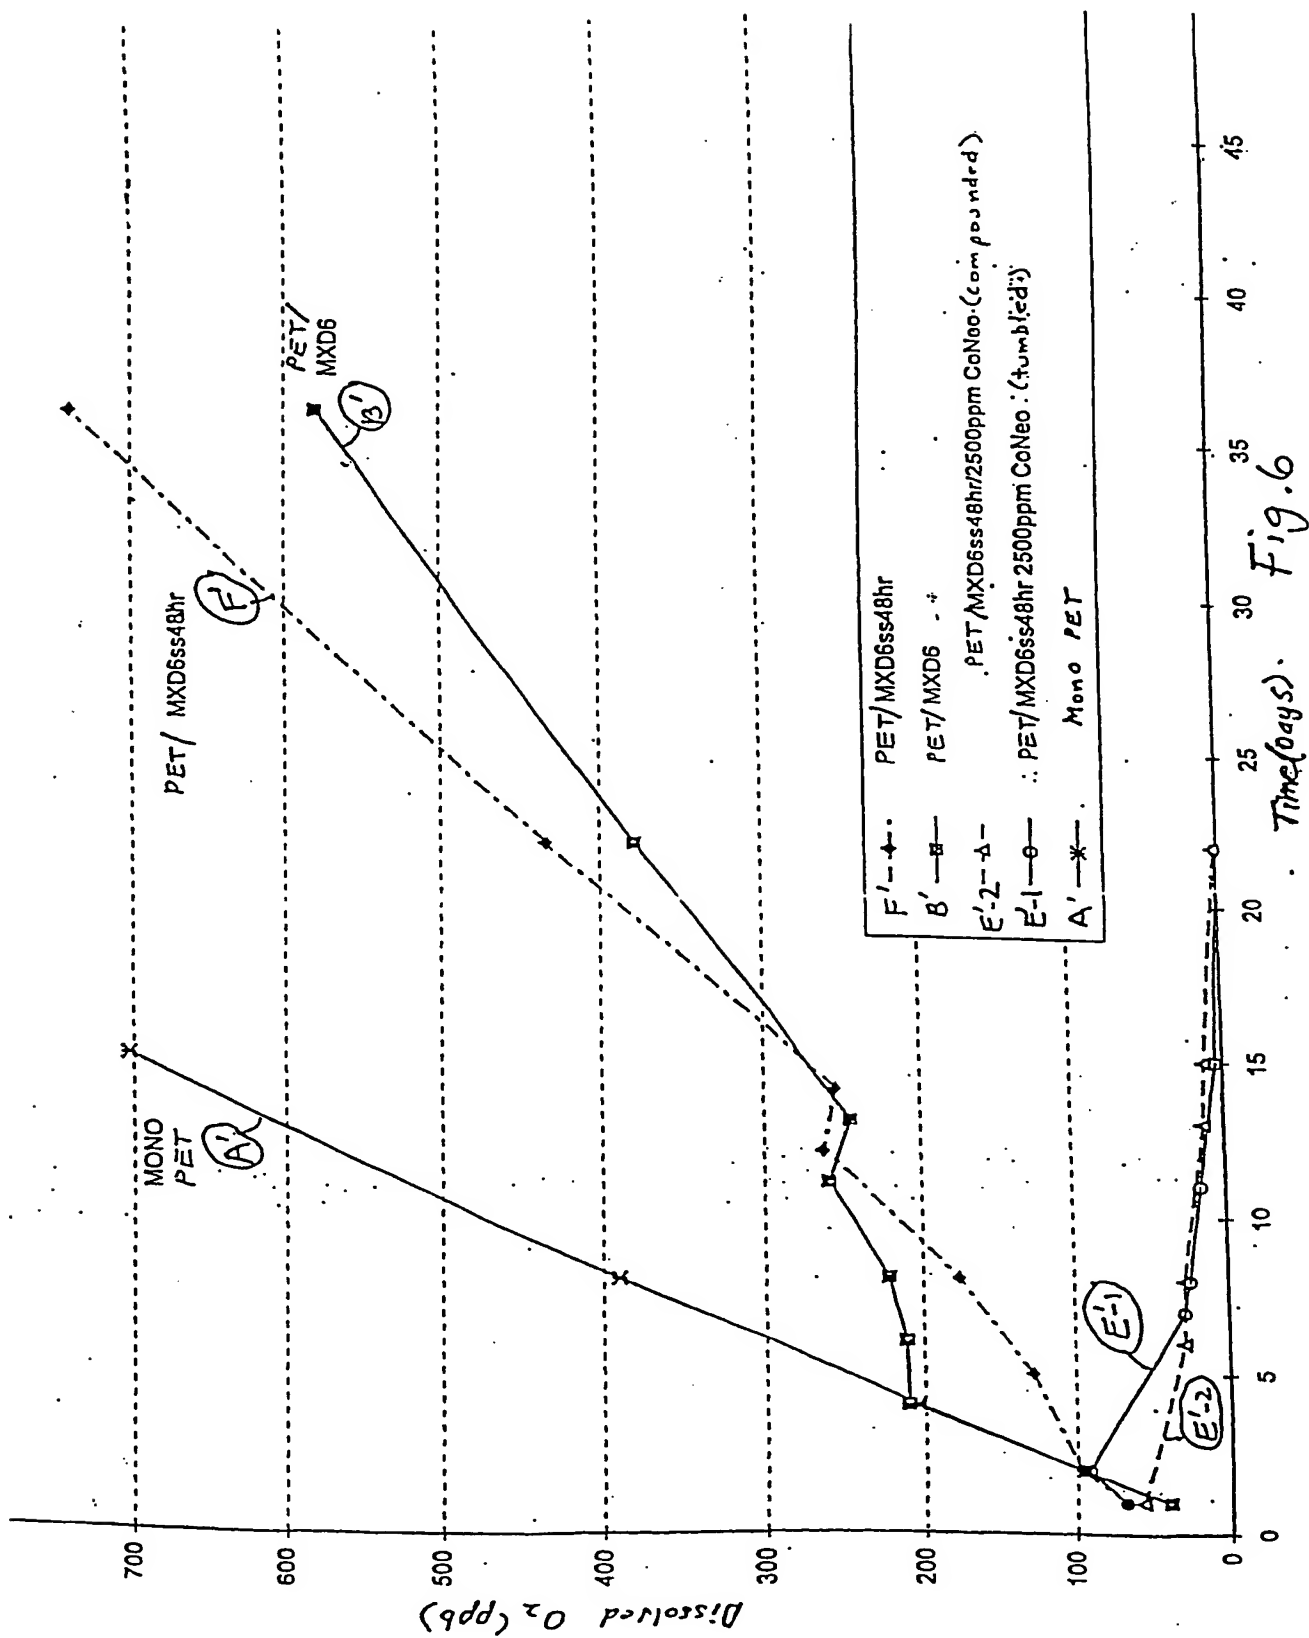


Fig. 6

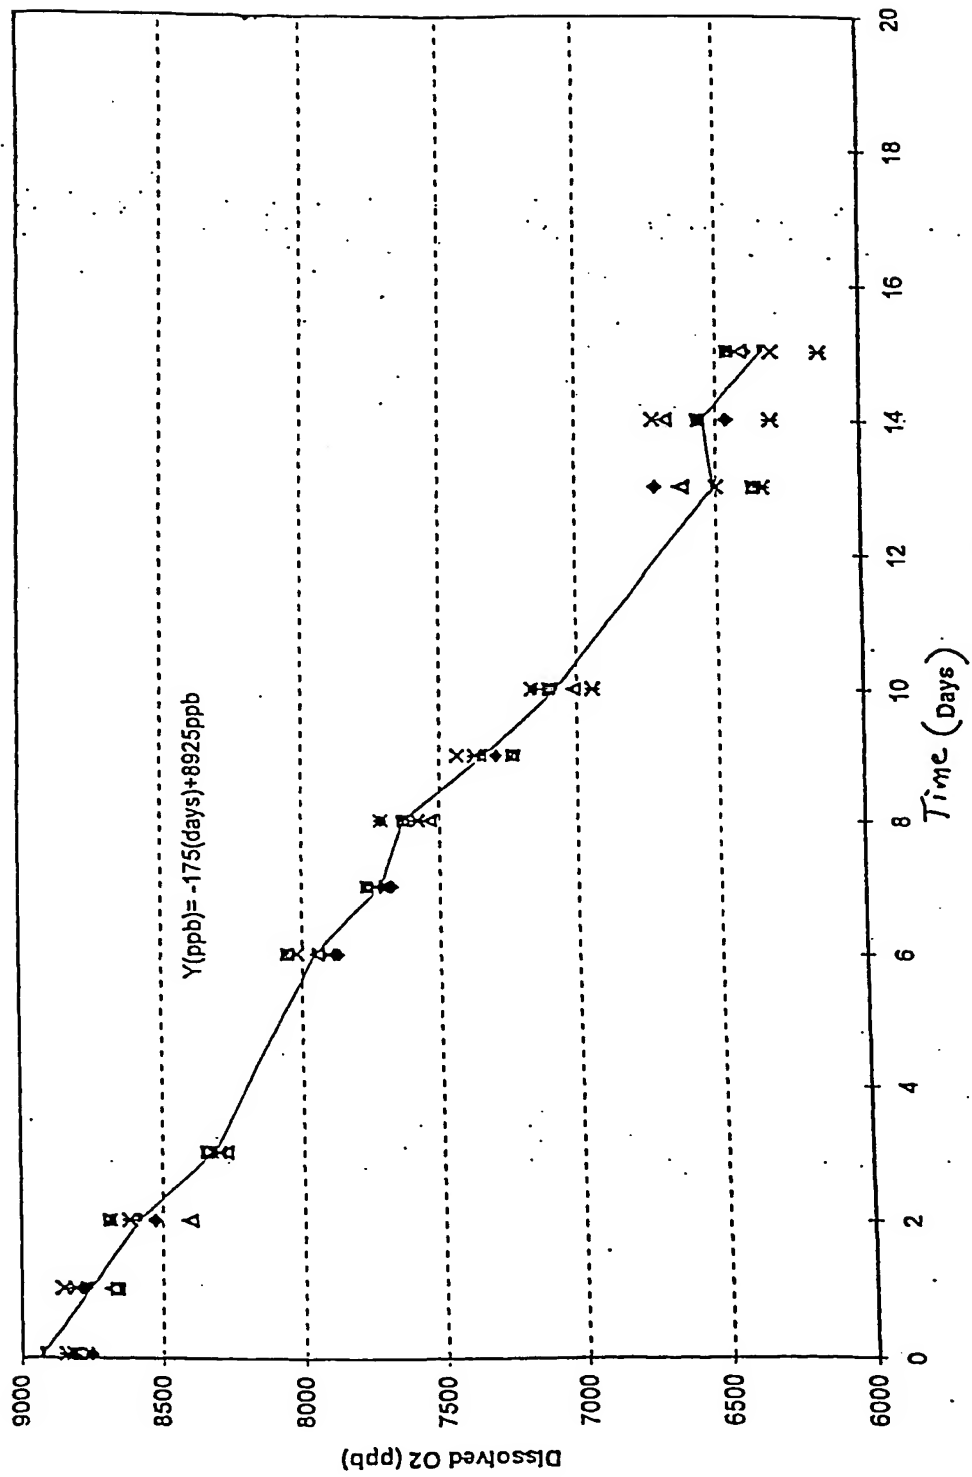


Fig. 7

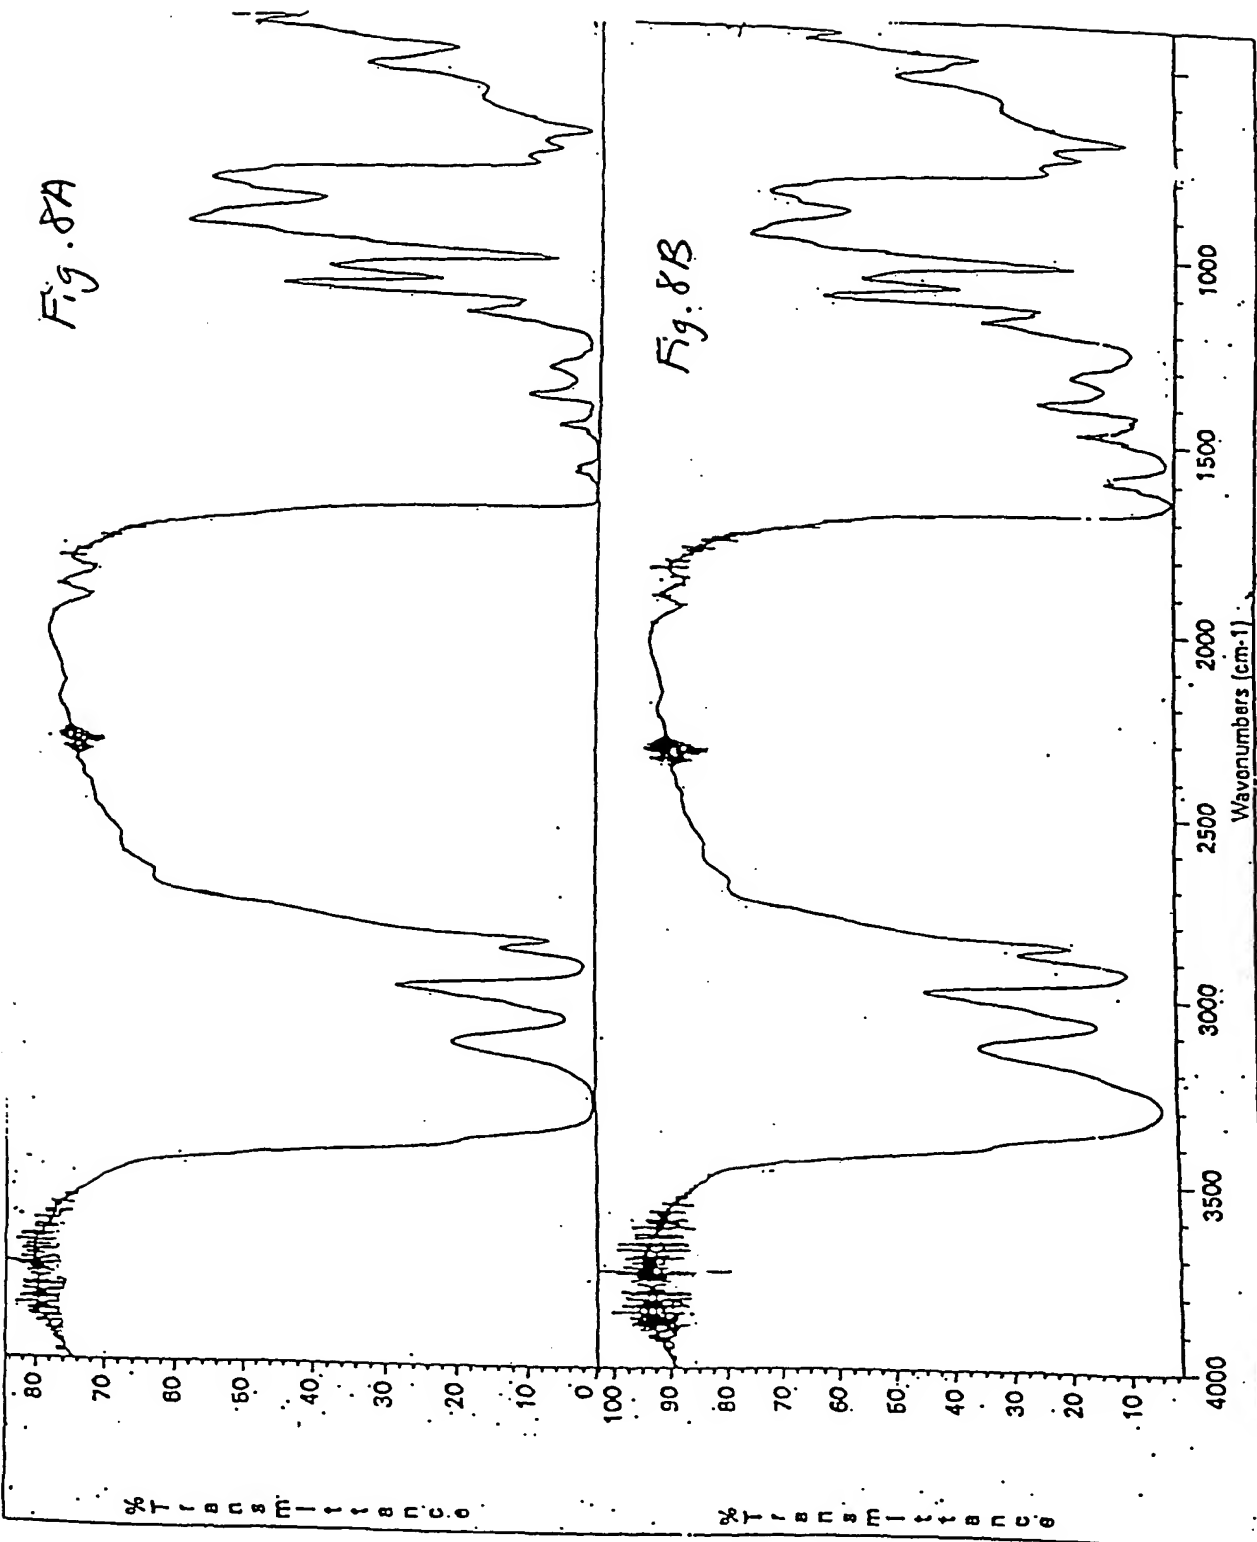


Fig. 9A

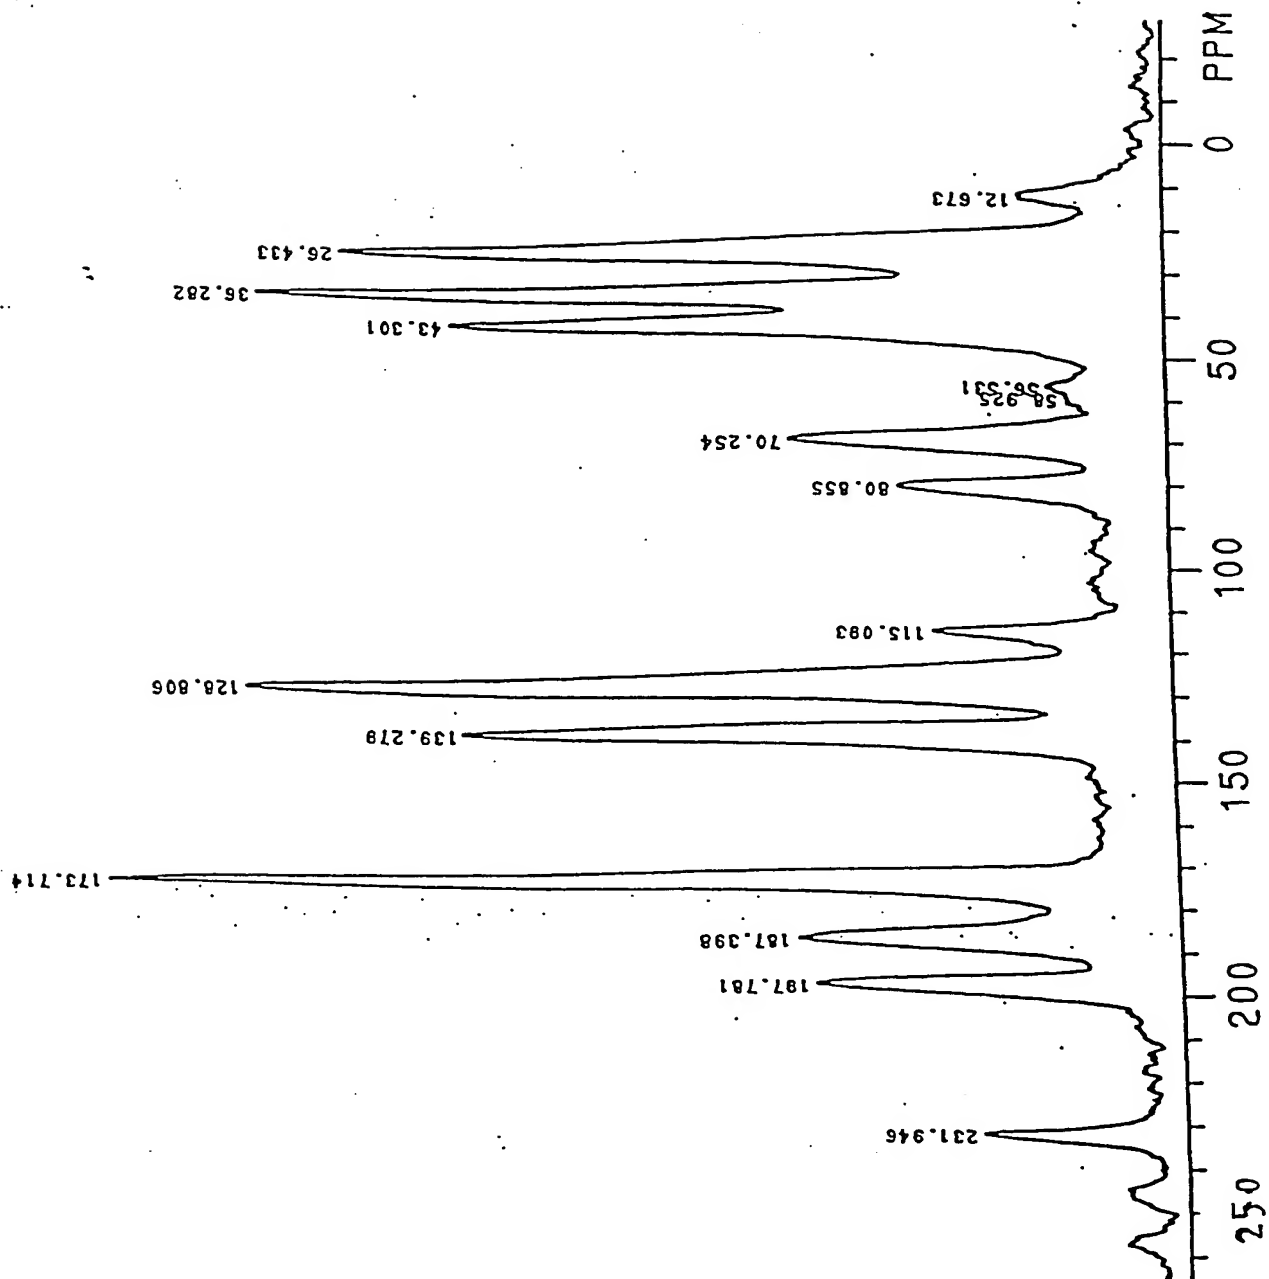


Fig. 9B

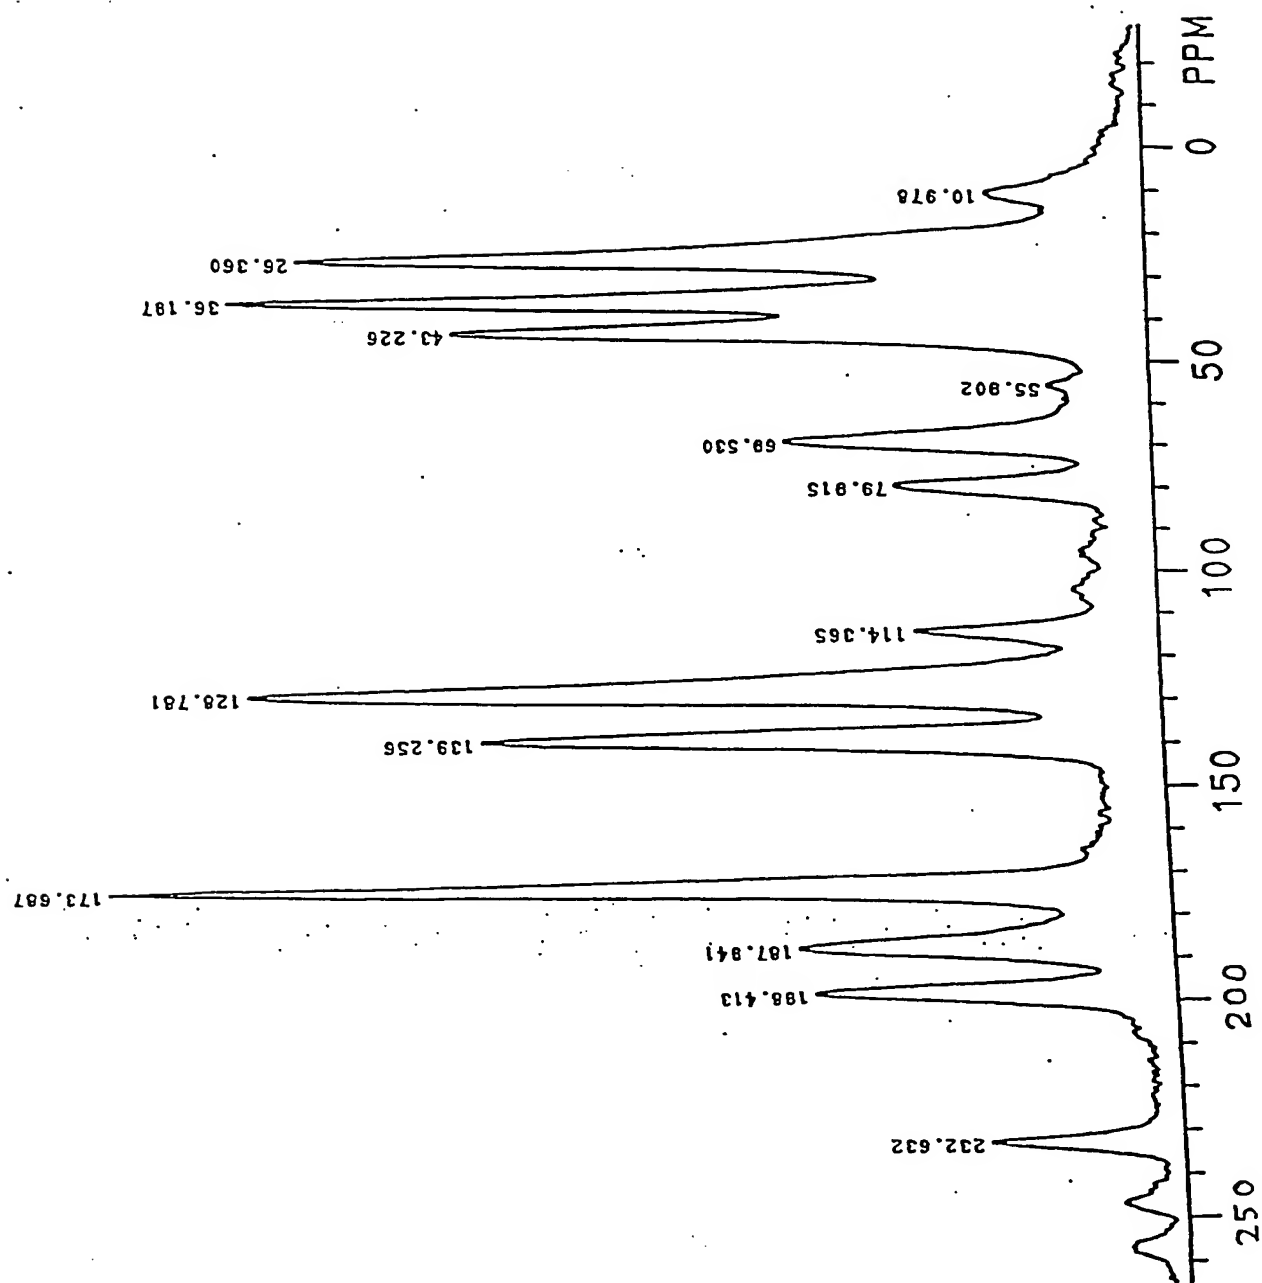
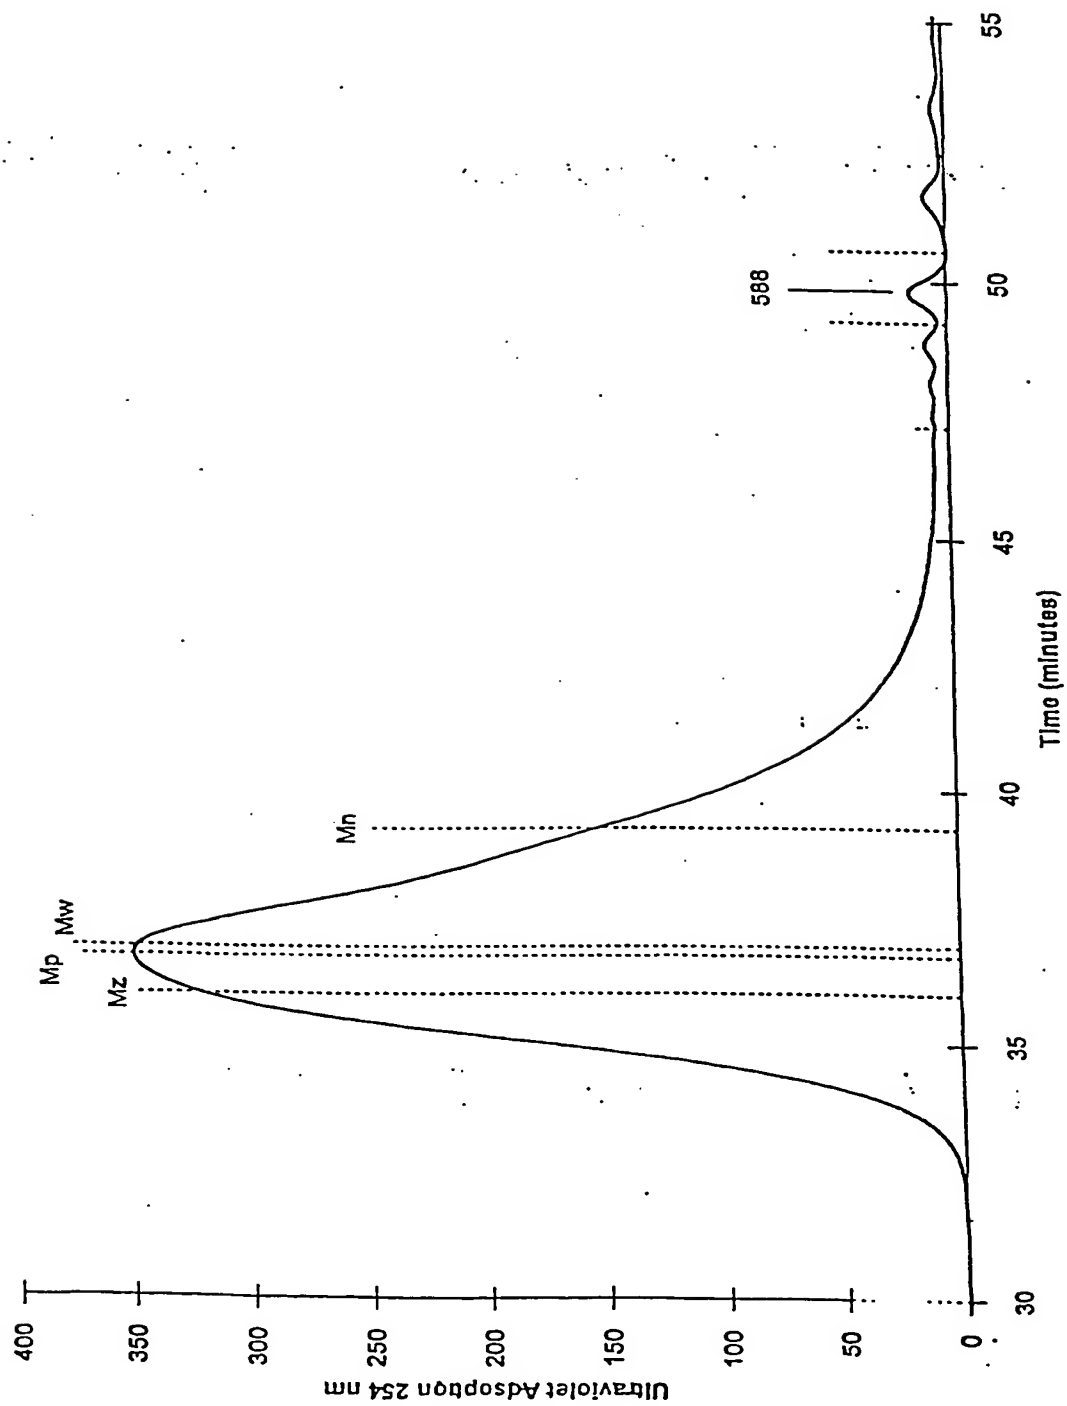




Fig. 10



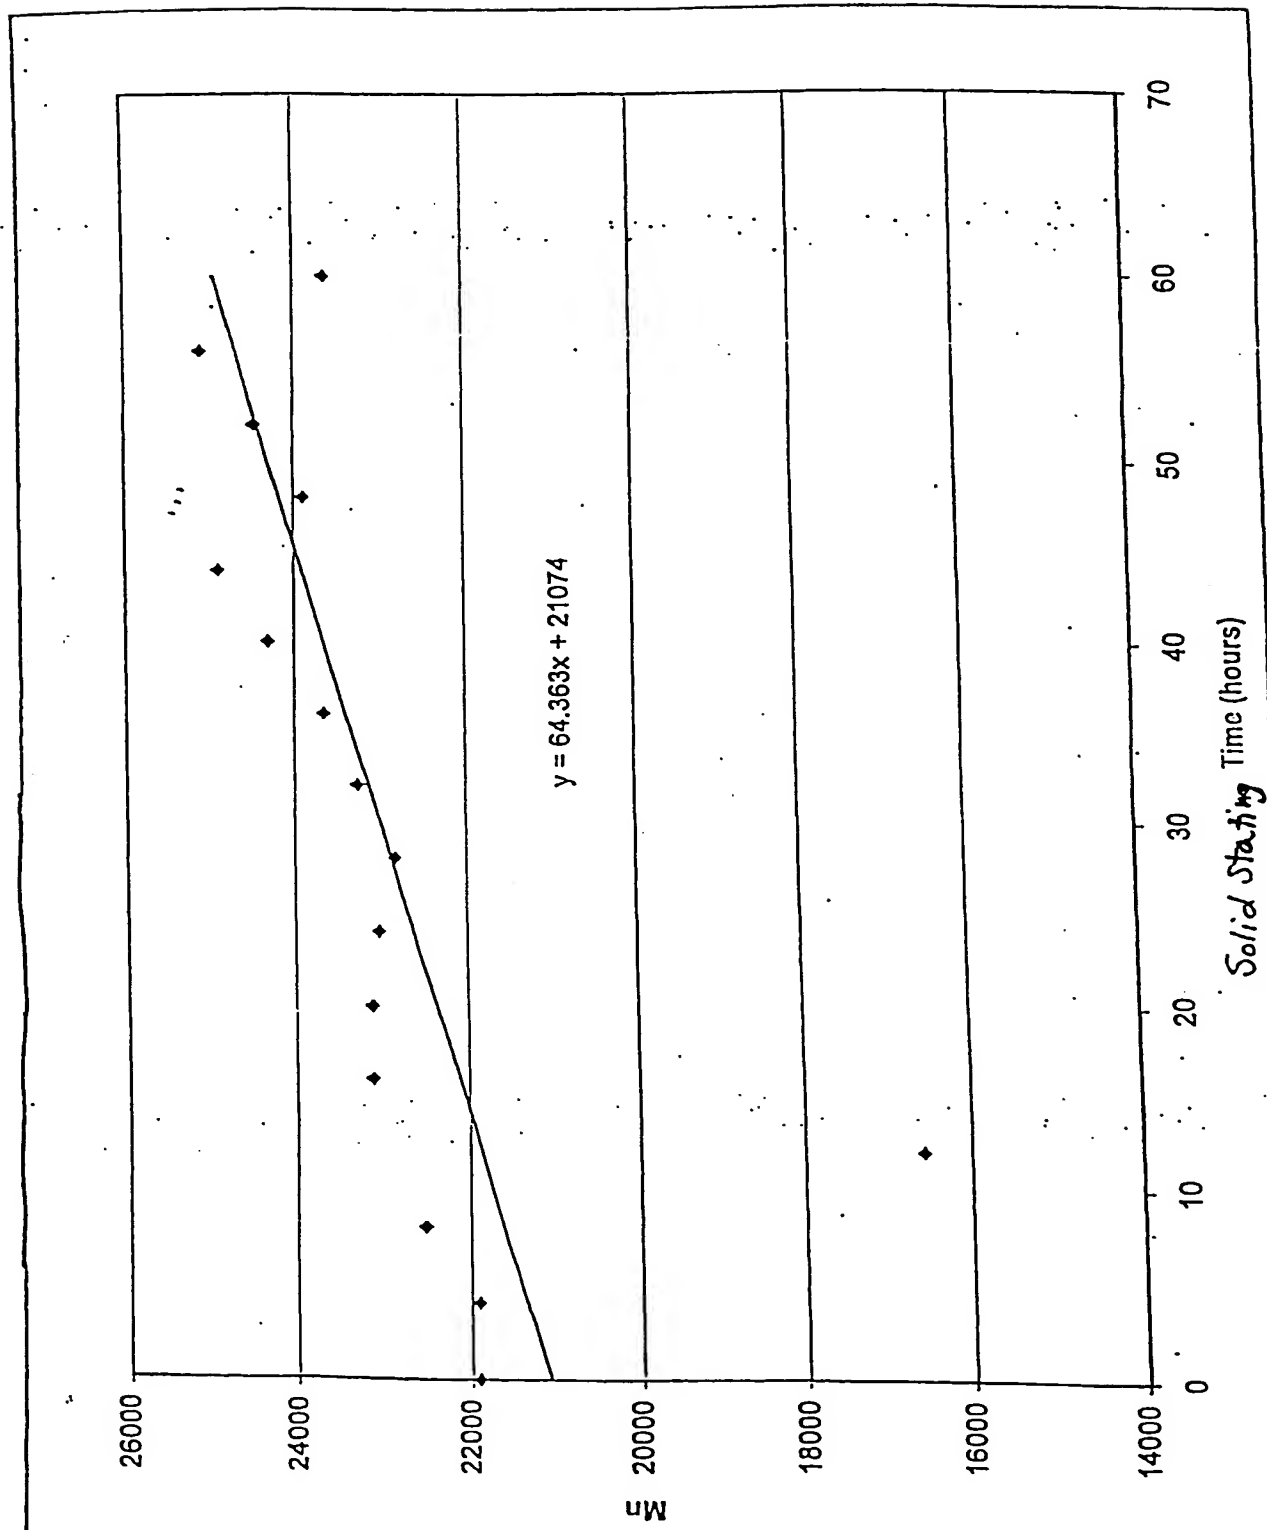


Fig. 11

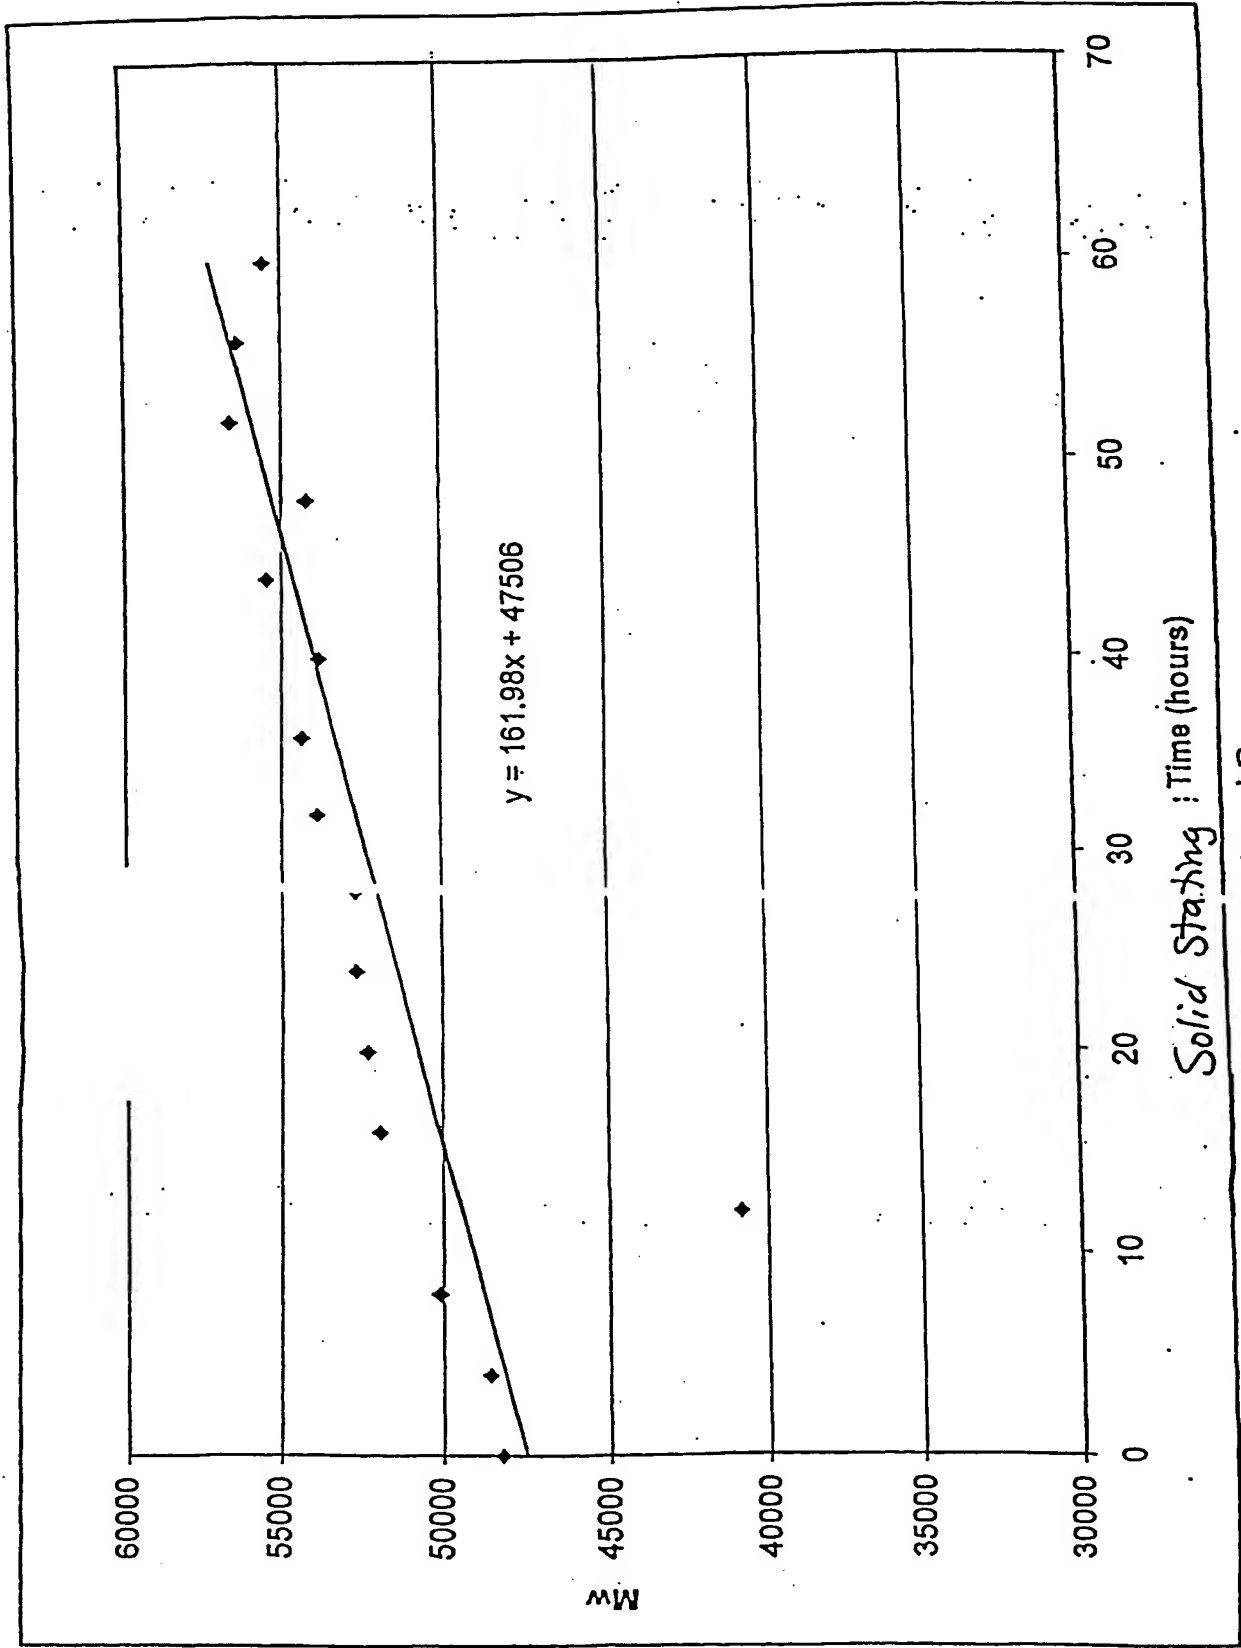


Fig. 12

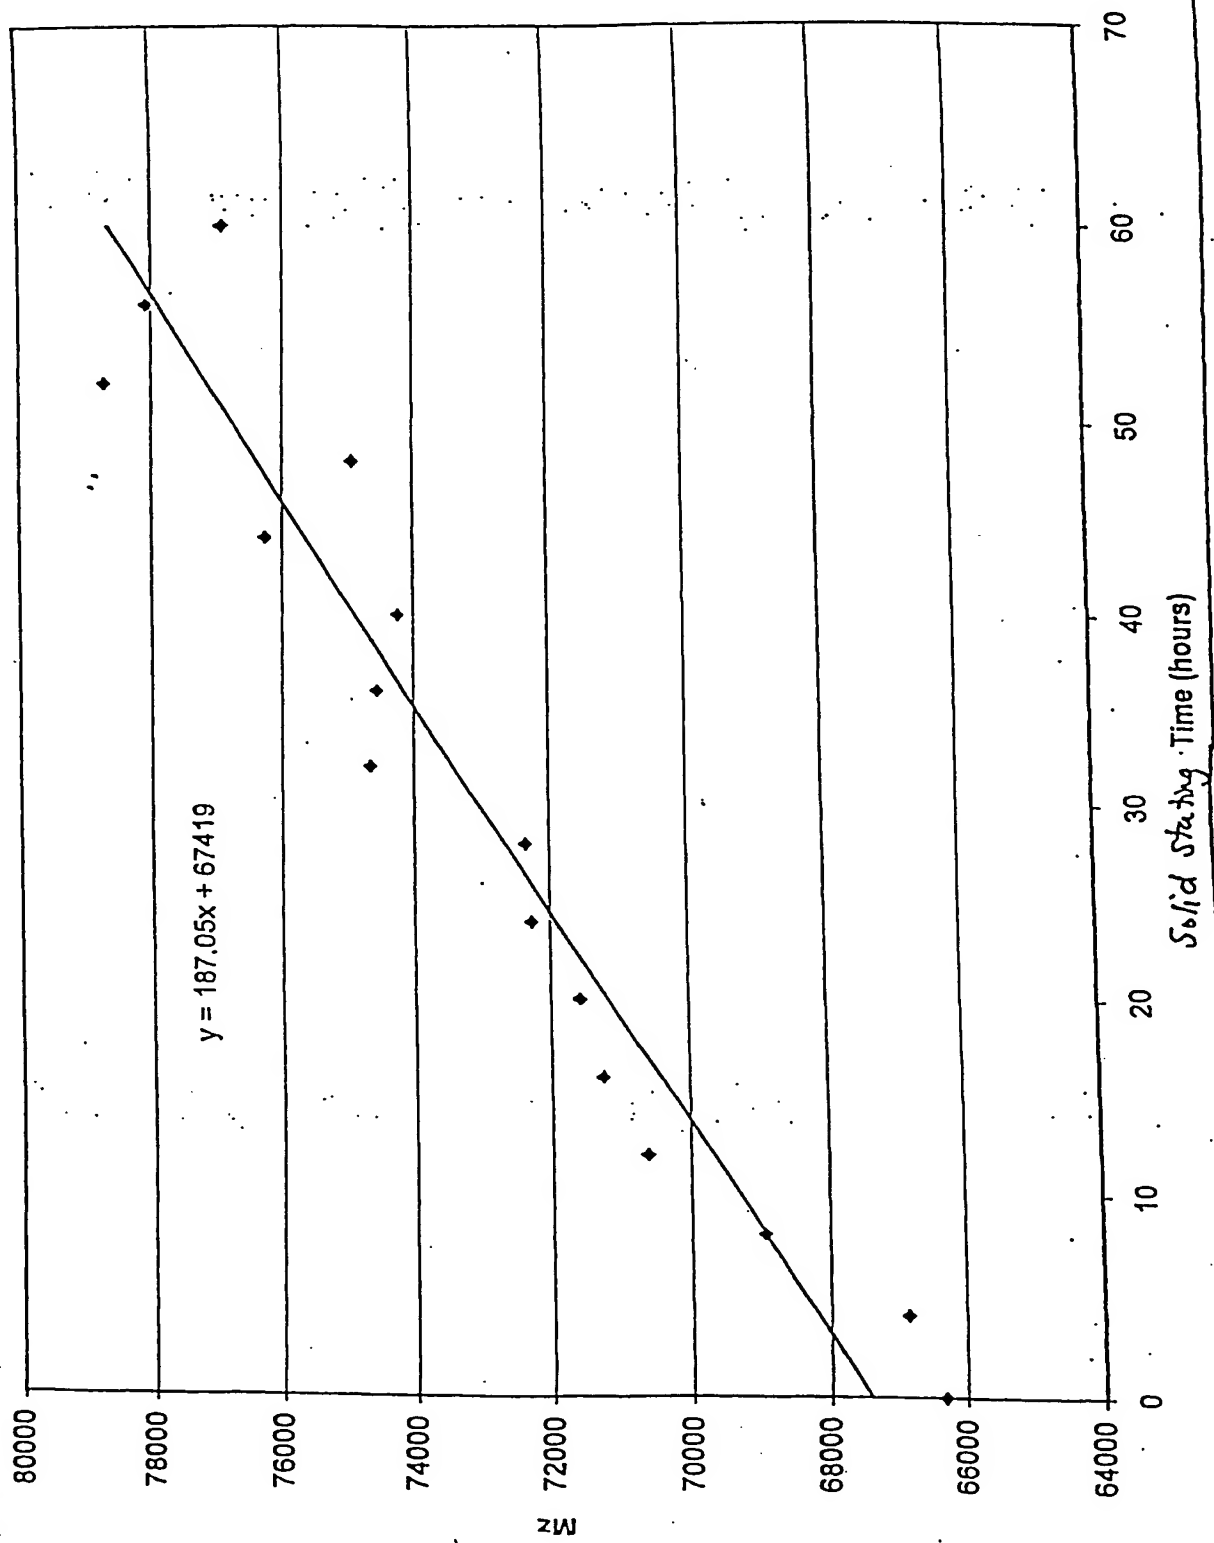
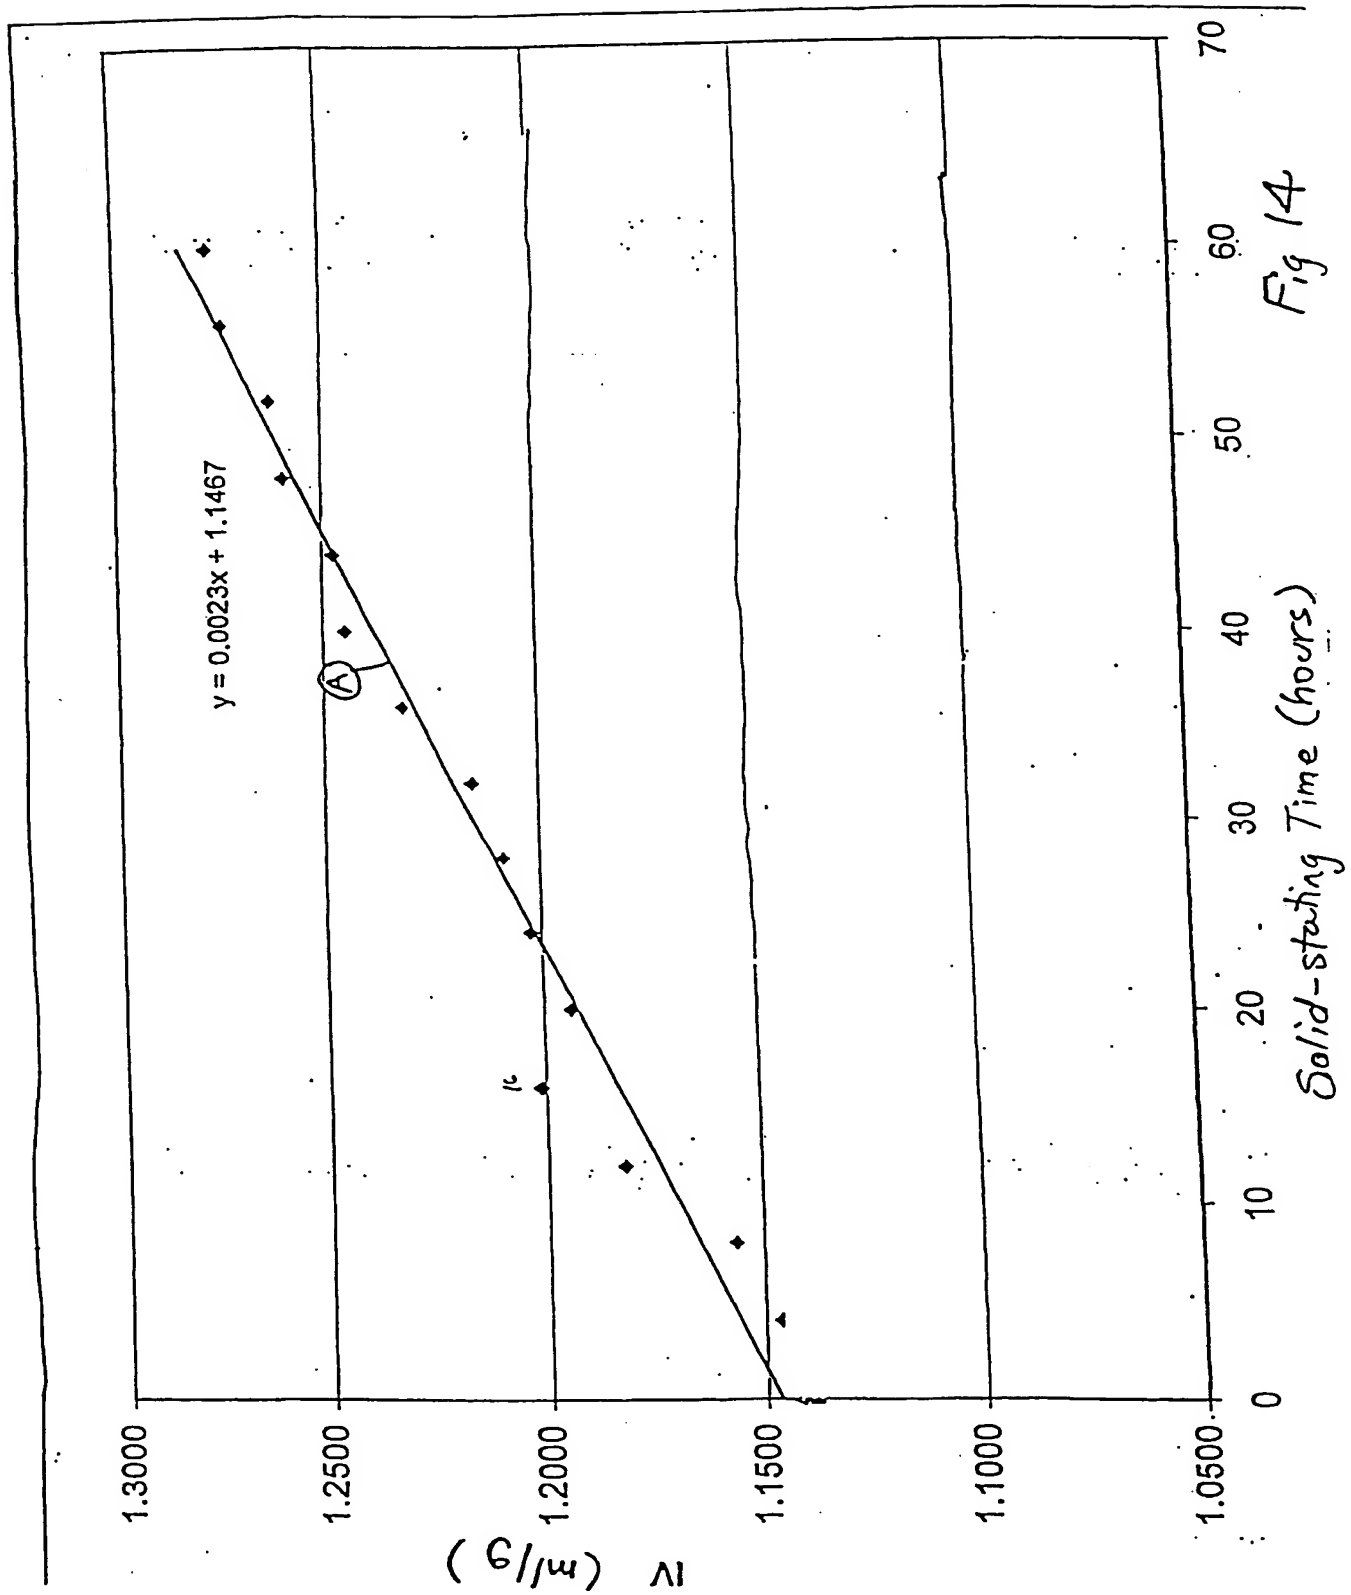


Fig. 13



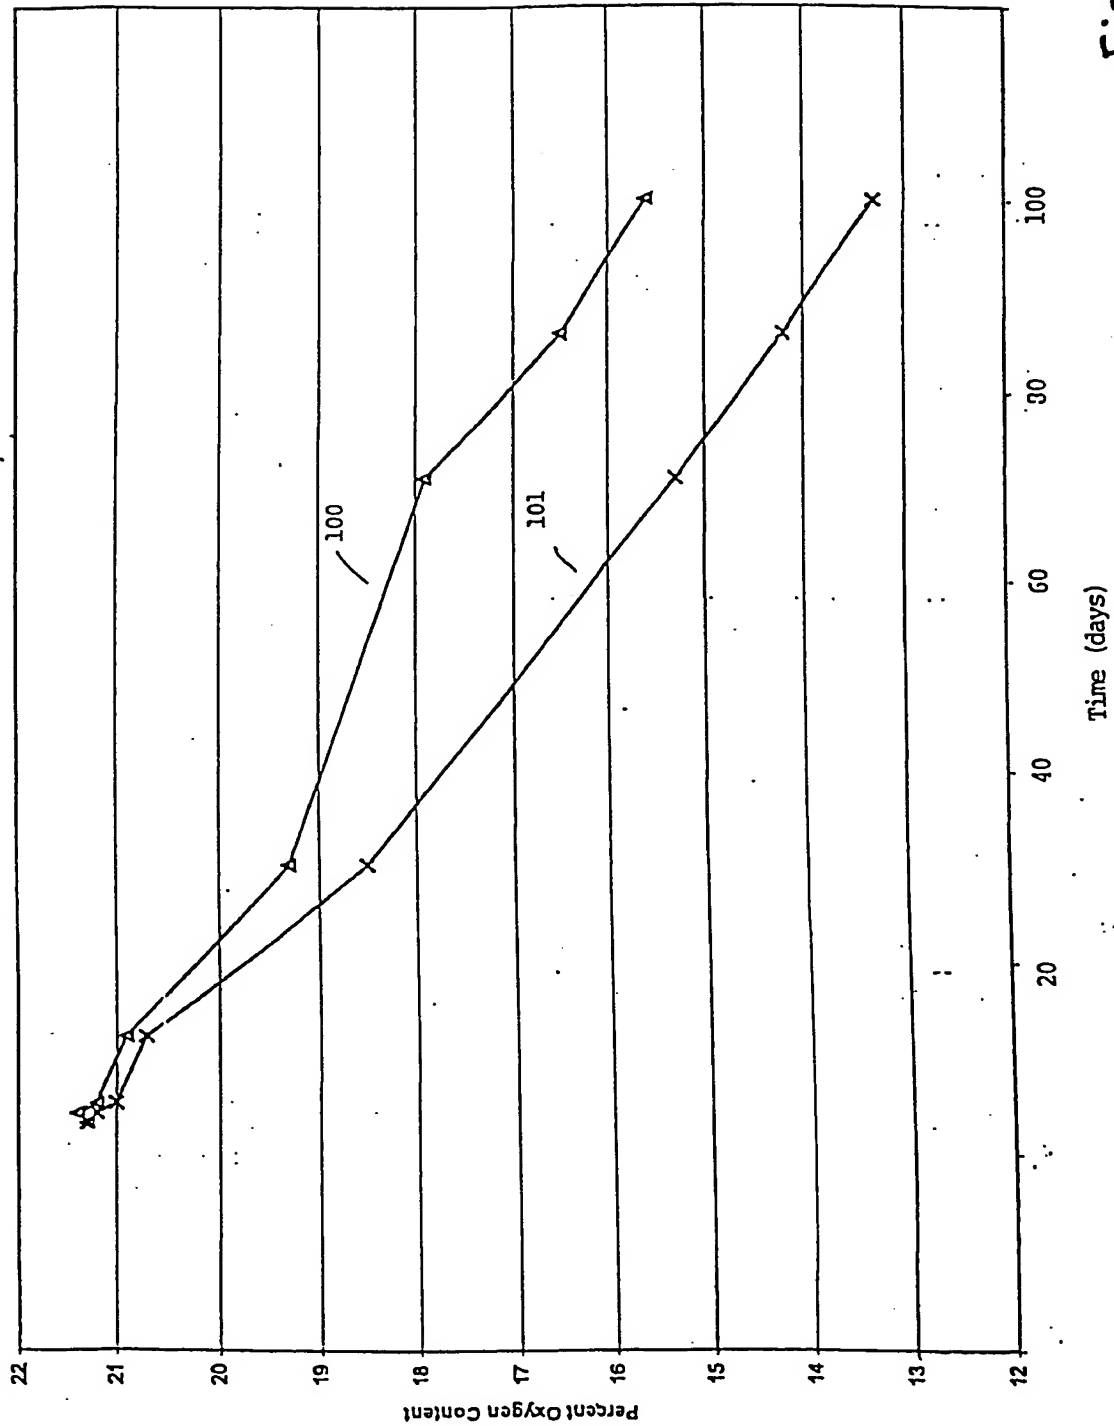


Fig. 15A

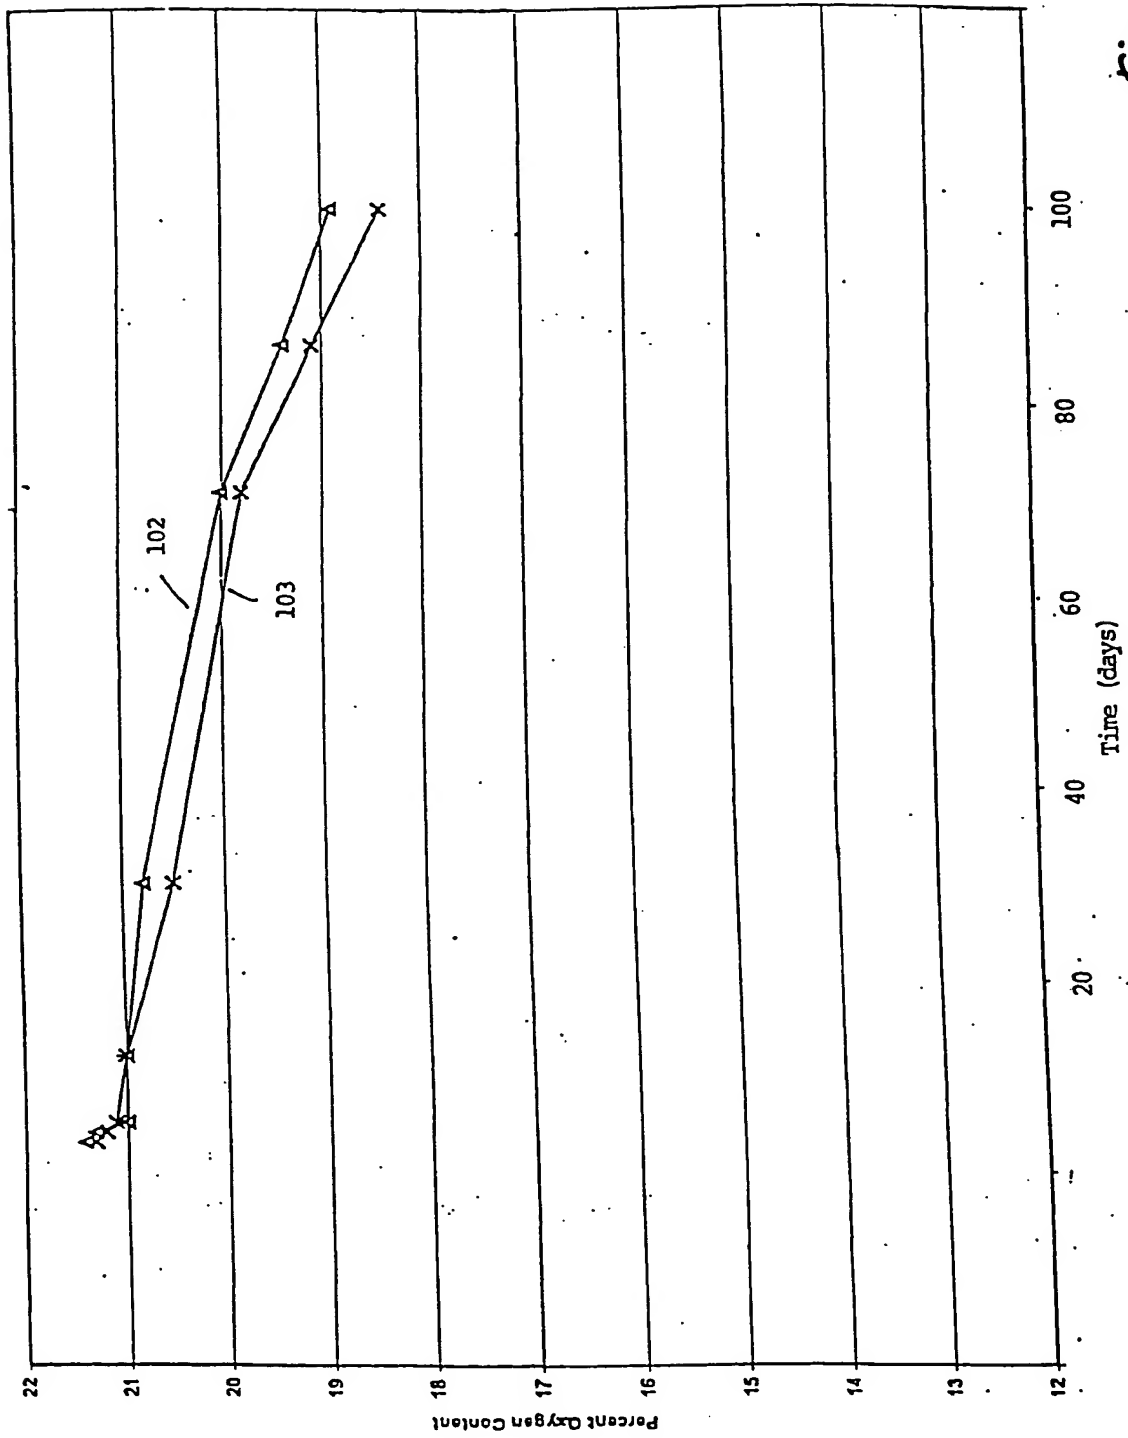


Fig 15B

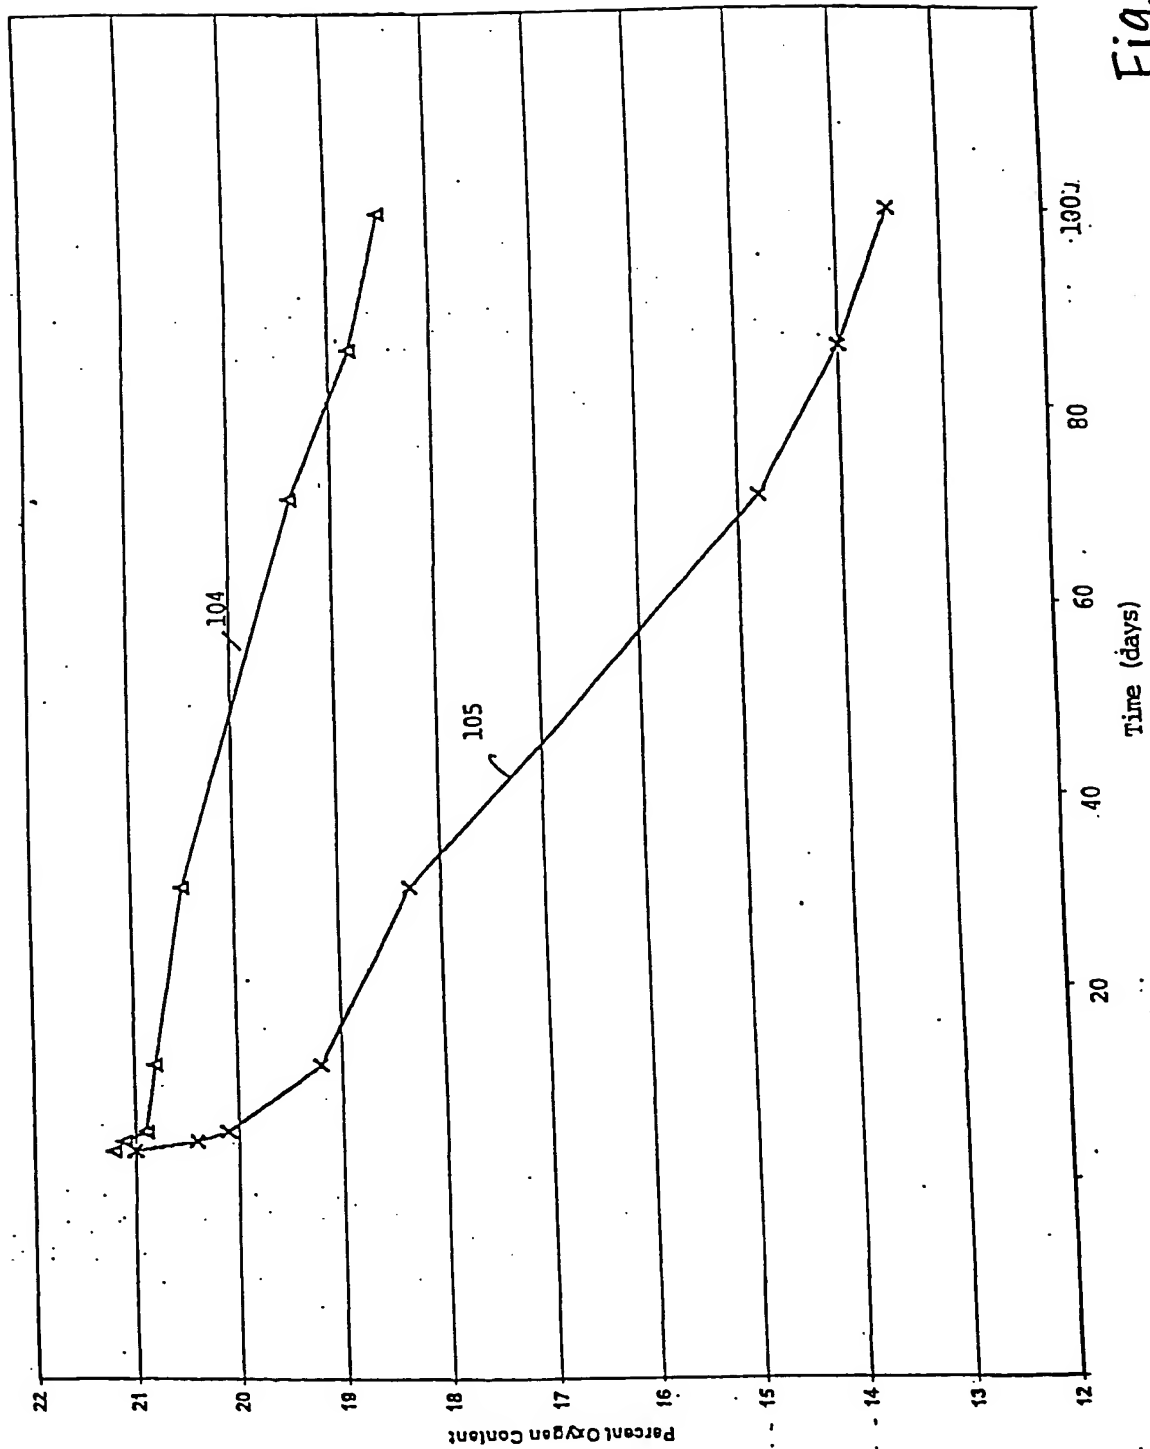


Fig. 15C



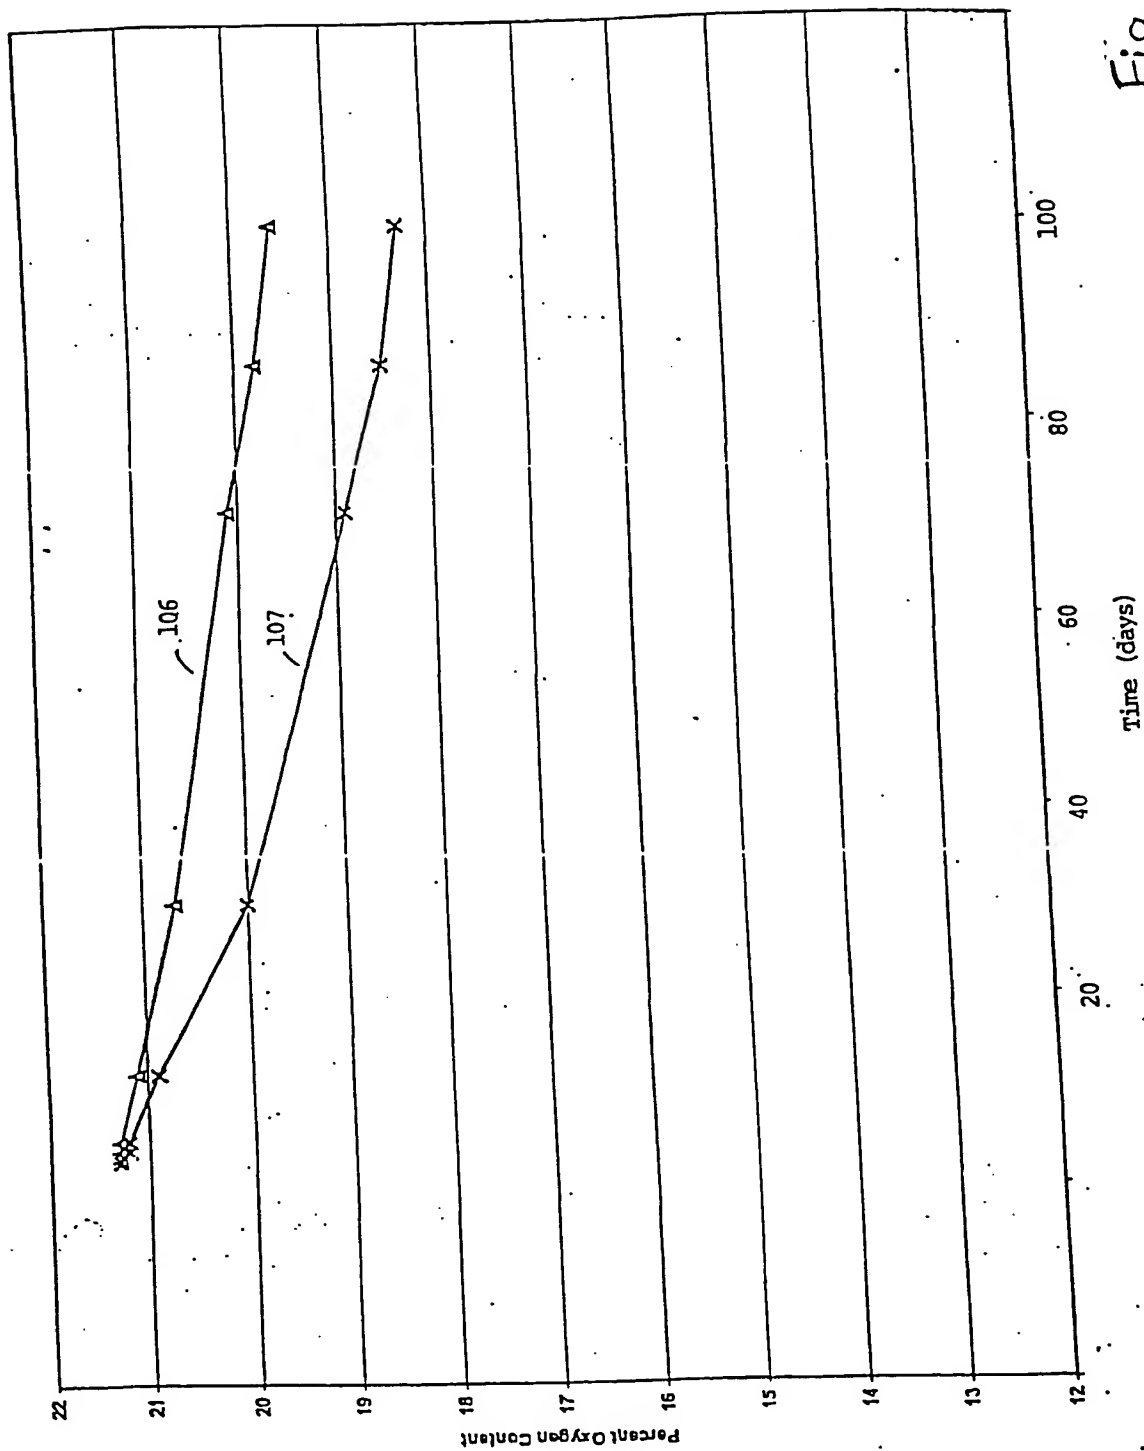



Fig 15D



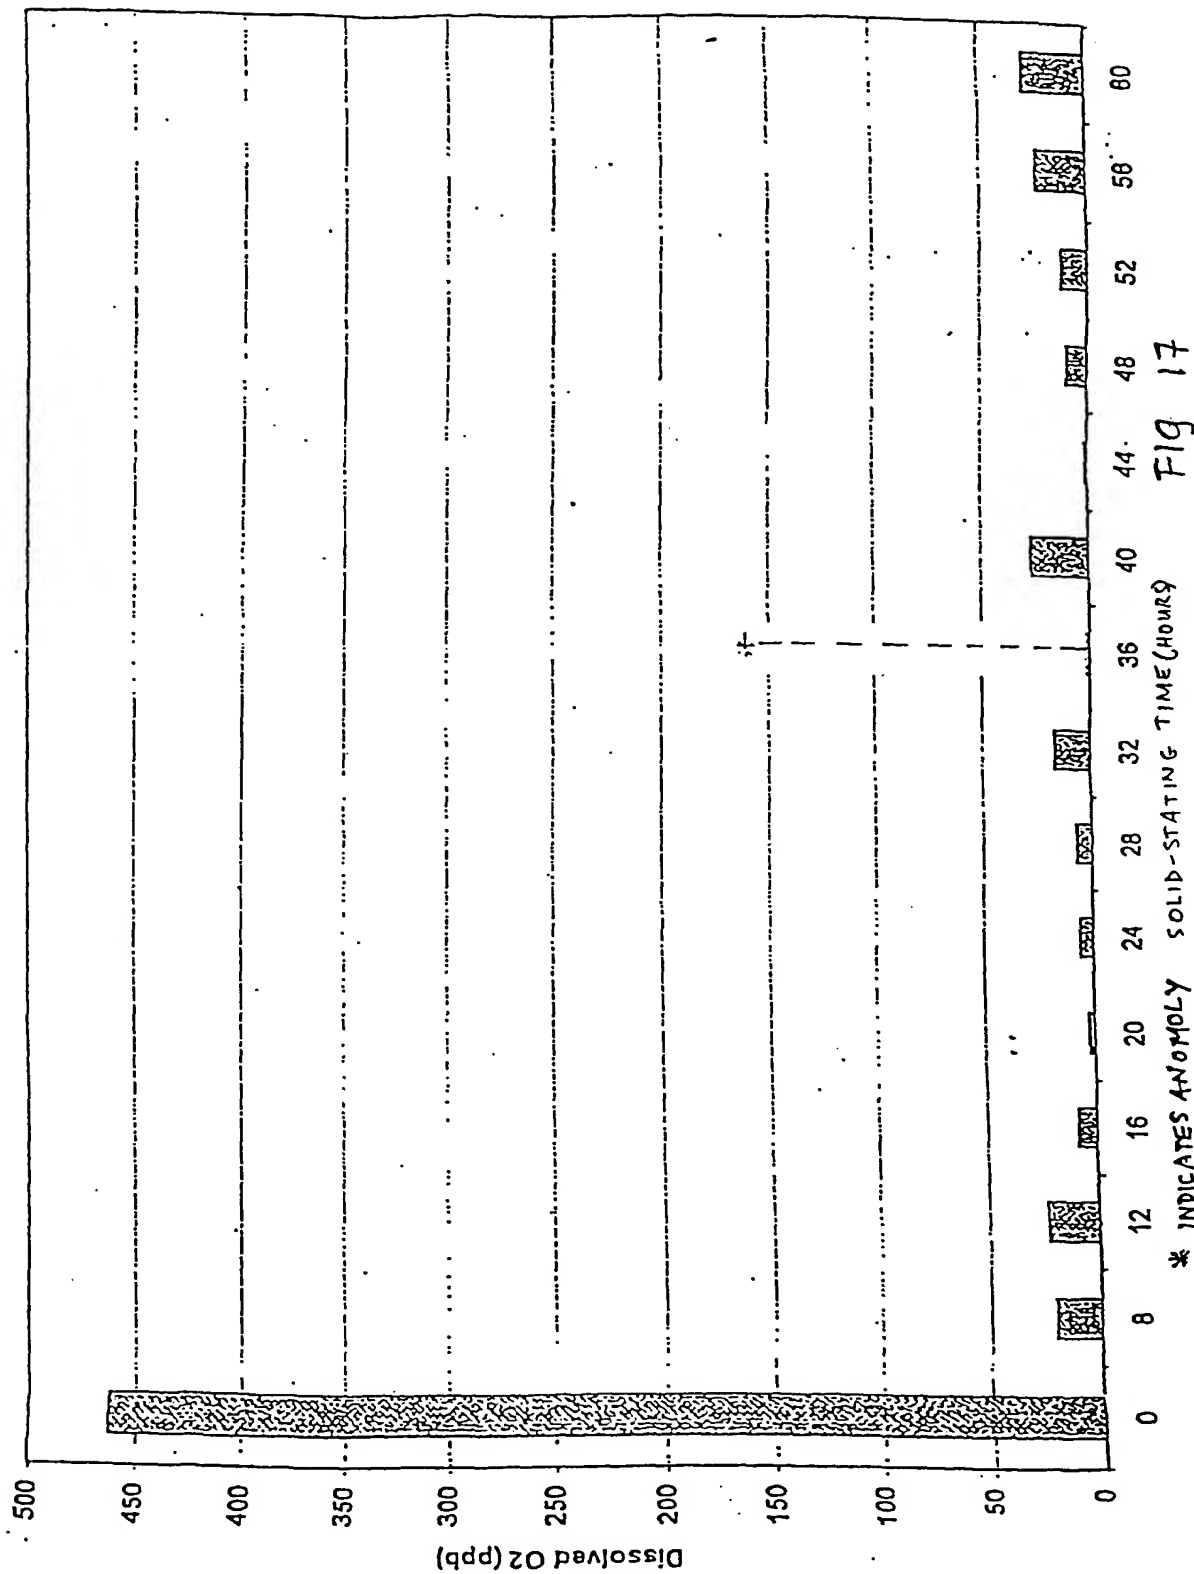


Fig 17

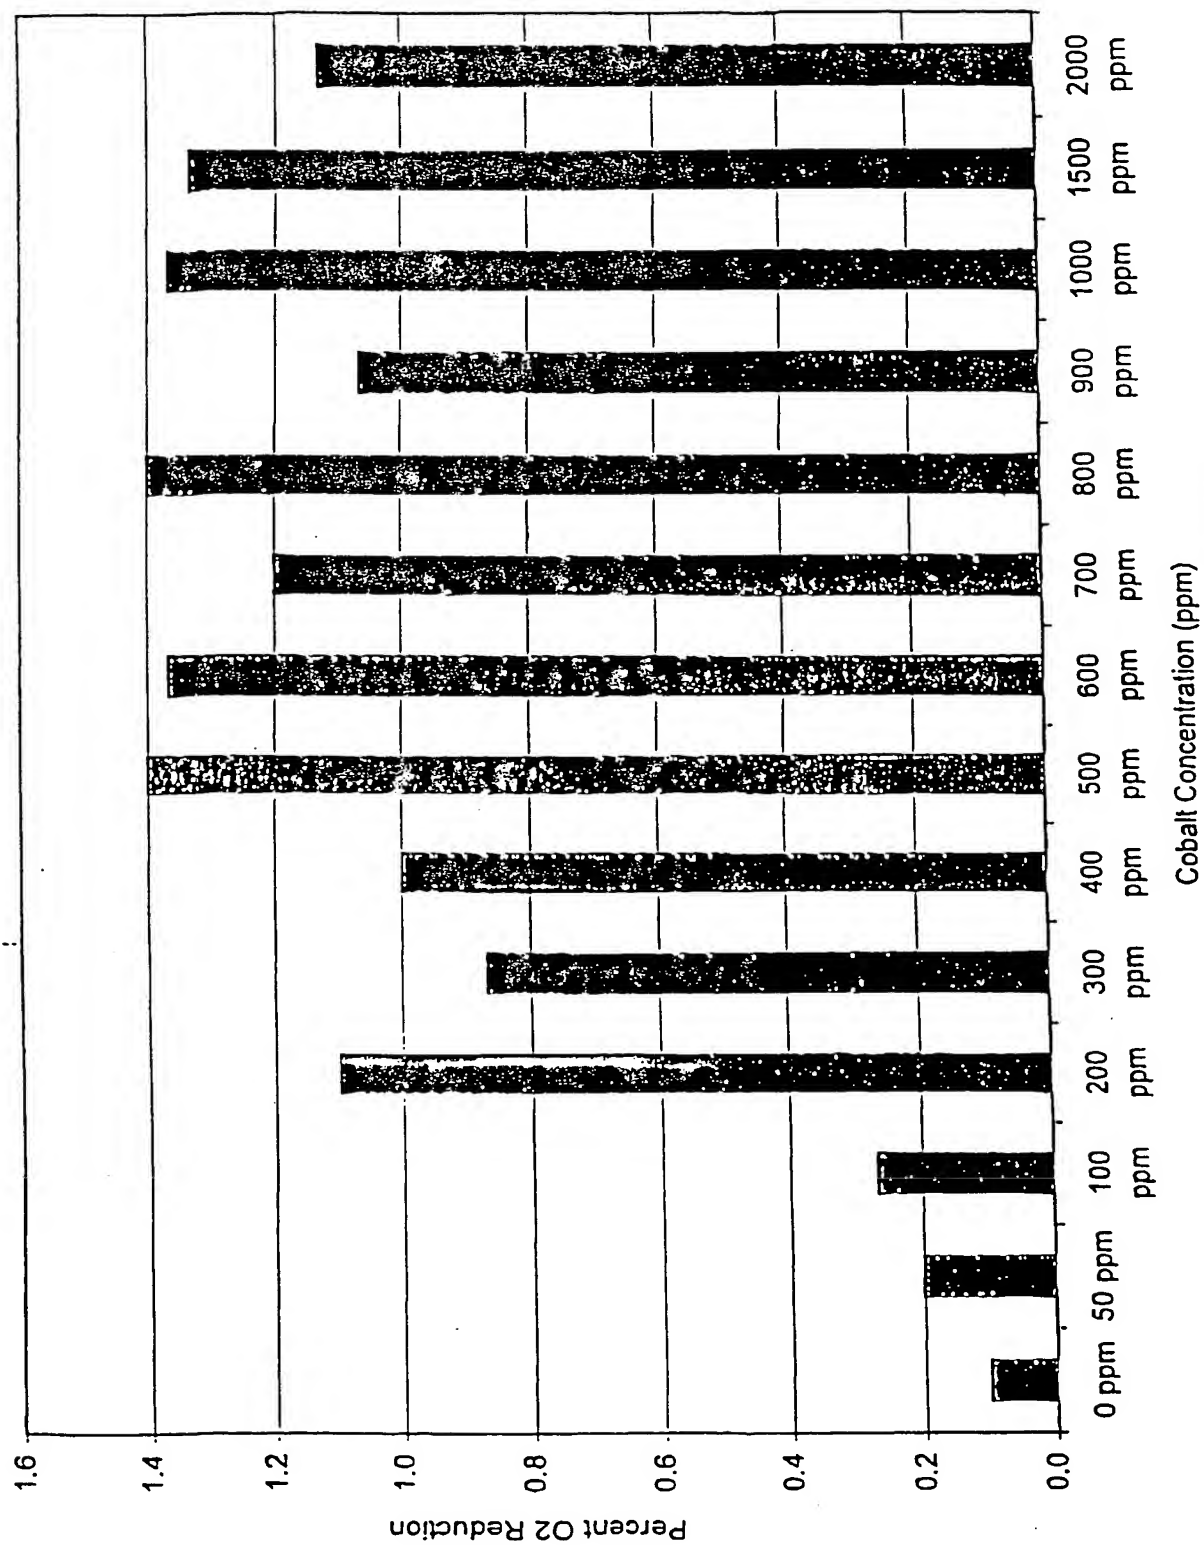


Fig. 18

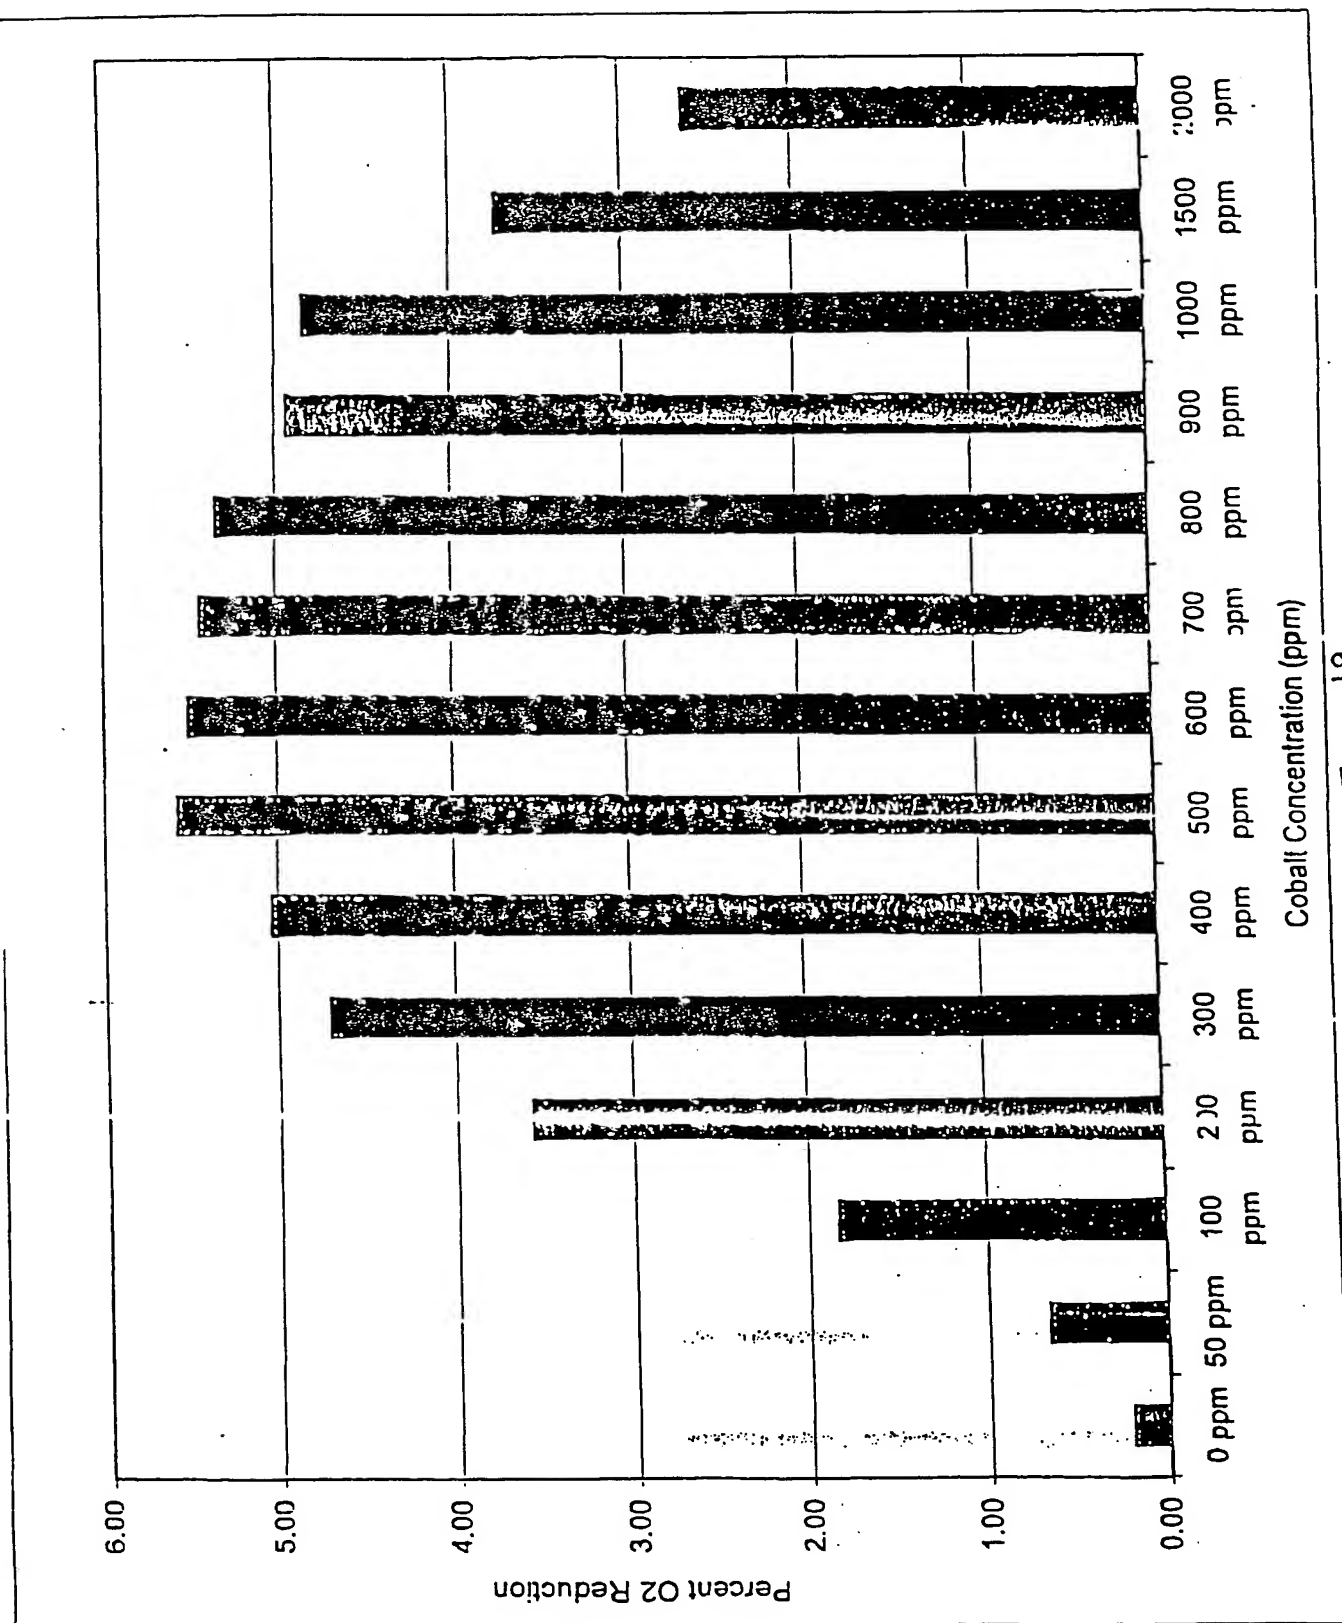


Fig. 19

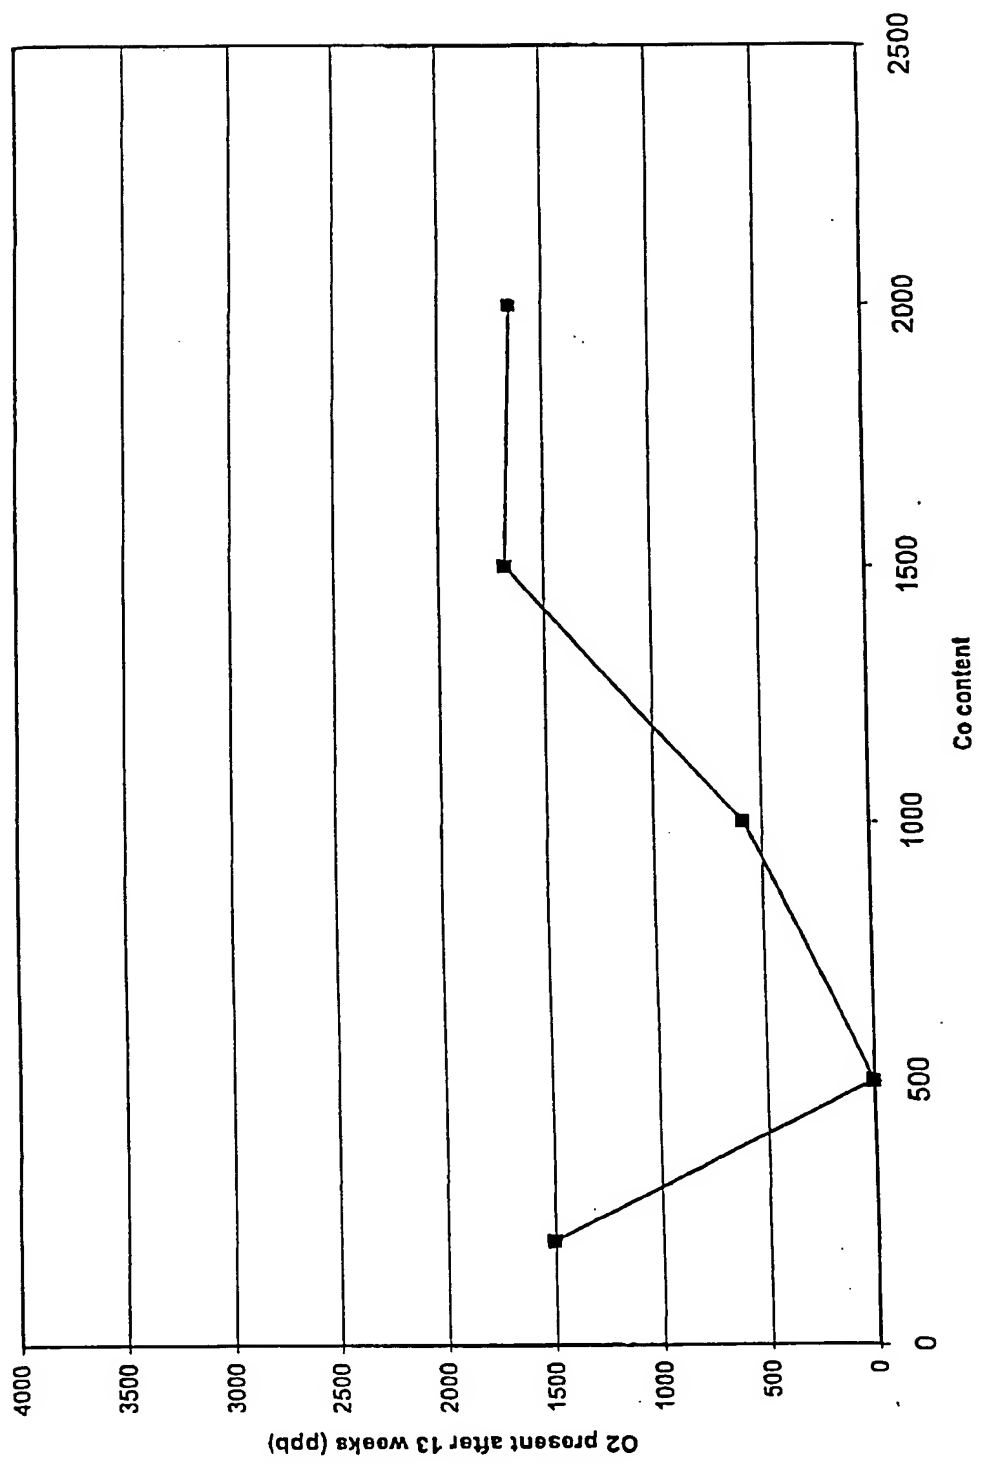
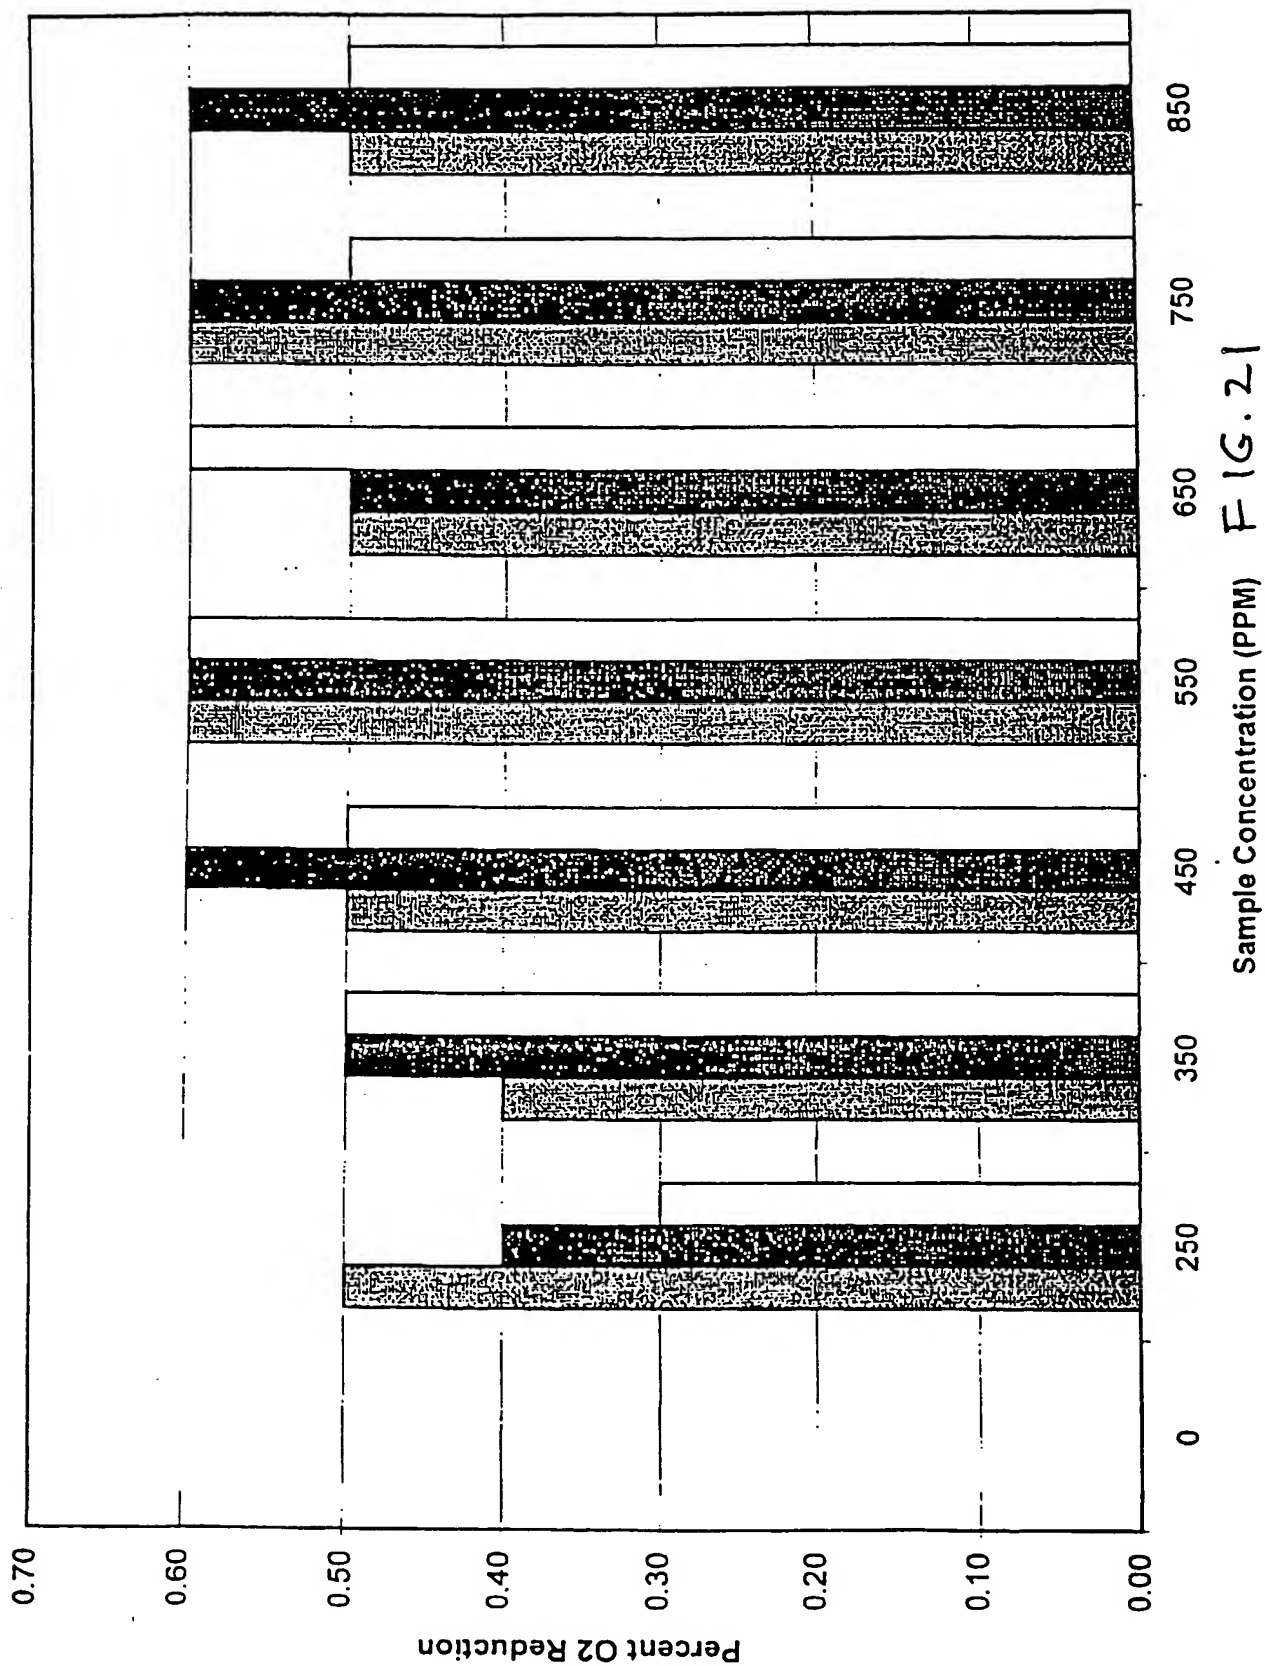


Fig. 20



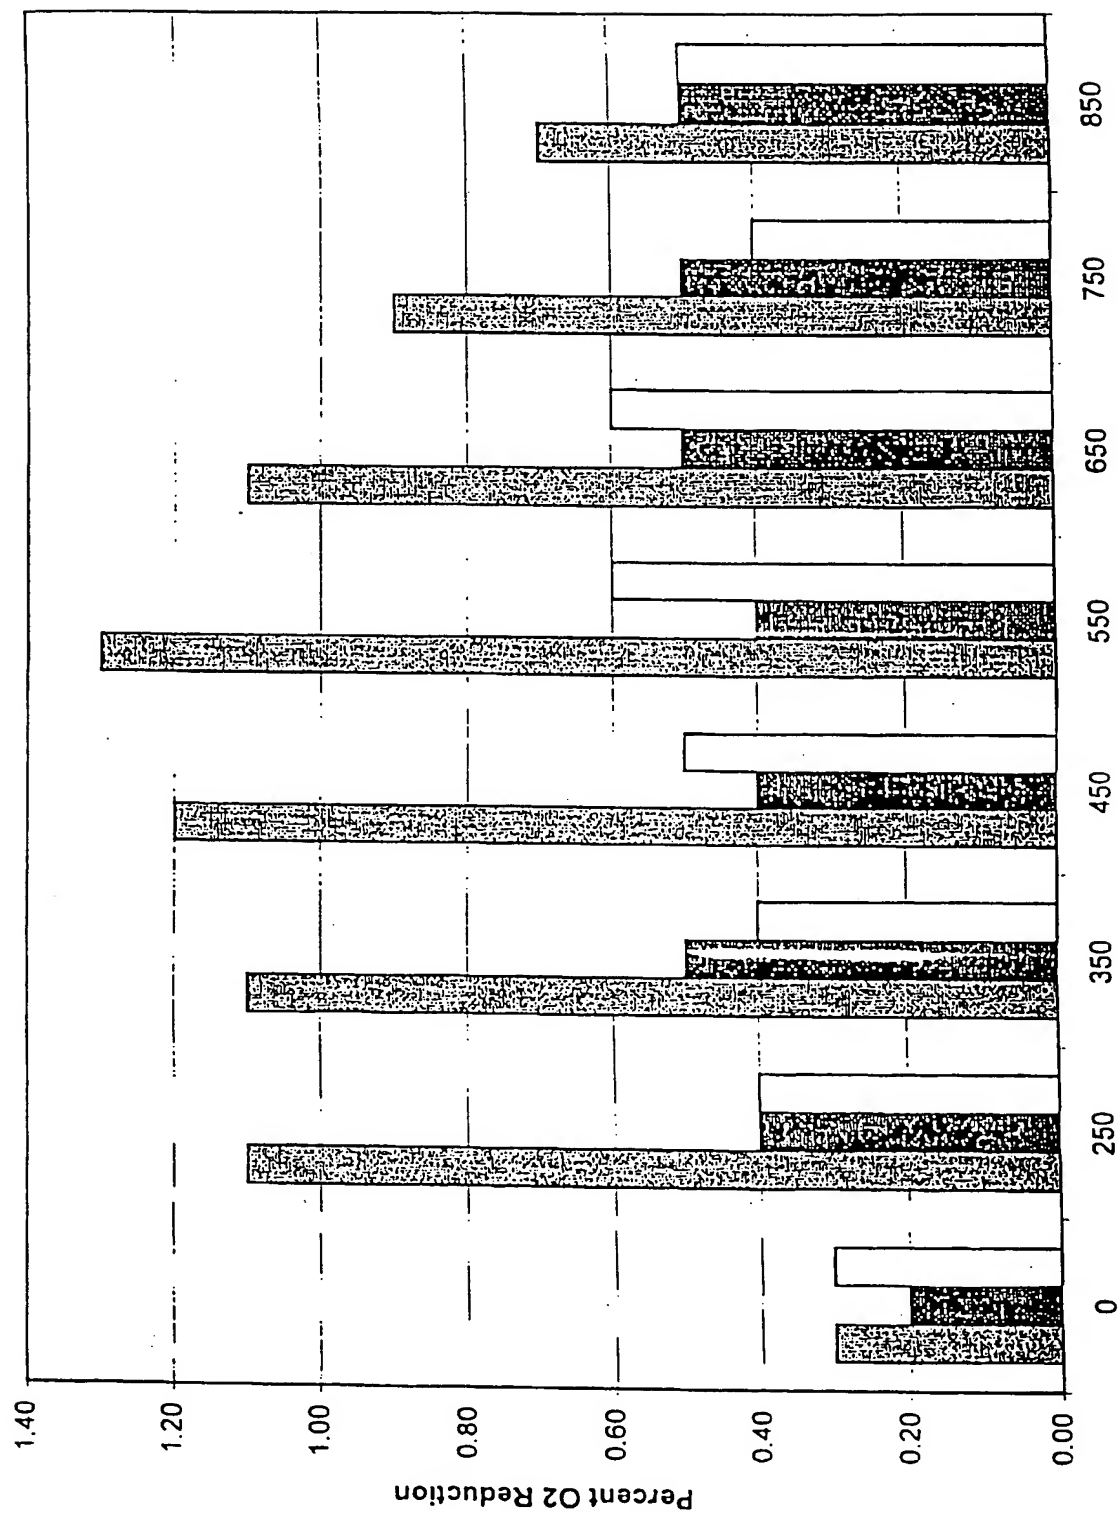


FIG. 22

Sample Concentration (PPM)